


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060519\
 Data File : BF114822.D
 Acq On : 5 Jun 2019 17:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 04 16:57:15 2019

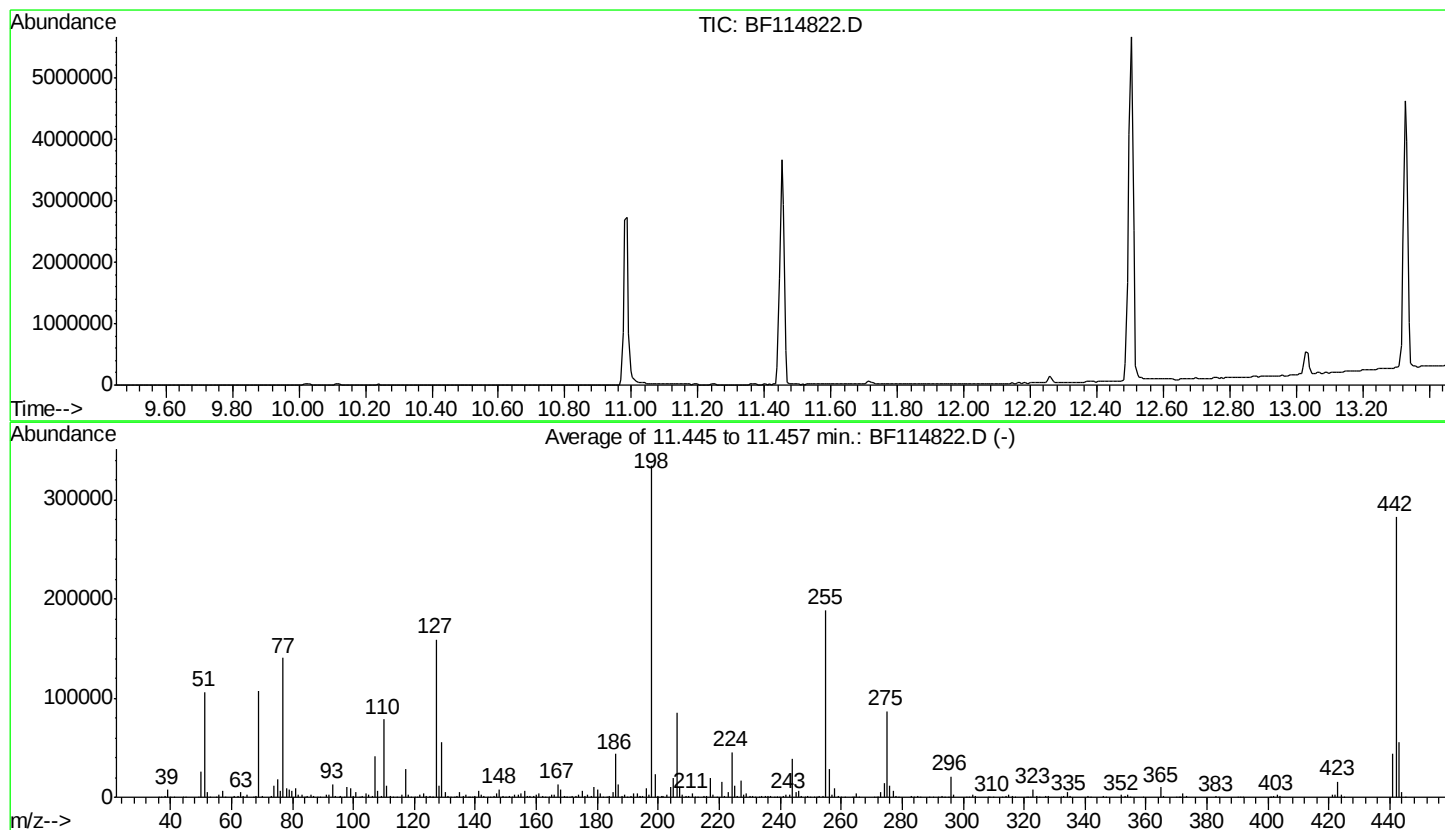

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	106384	PASS
68	69	0.00	2	1.3	1398	PASS
69	198	0.00	100	32.0	107100	PASS
70	69	0.00	2	0.7	771	PASS
127	198	10	80	47.6	159114	PASS
197	198	0.00	2	0.7	2292	PASS
198	198	100	100	100.0	334229	PASS
199	198	5	9	6.8	22832	PASS
275	198	10	60	25.9	86528	PASS
365	198	1	100	2.9	9859	PASS
441	198	0.01	100	13.3	44304	PASS
442	198	50	100	84.6	282714	PASS
443	442	15	24	19.8	55981	PASS