
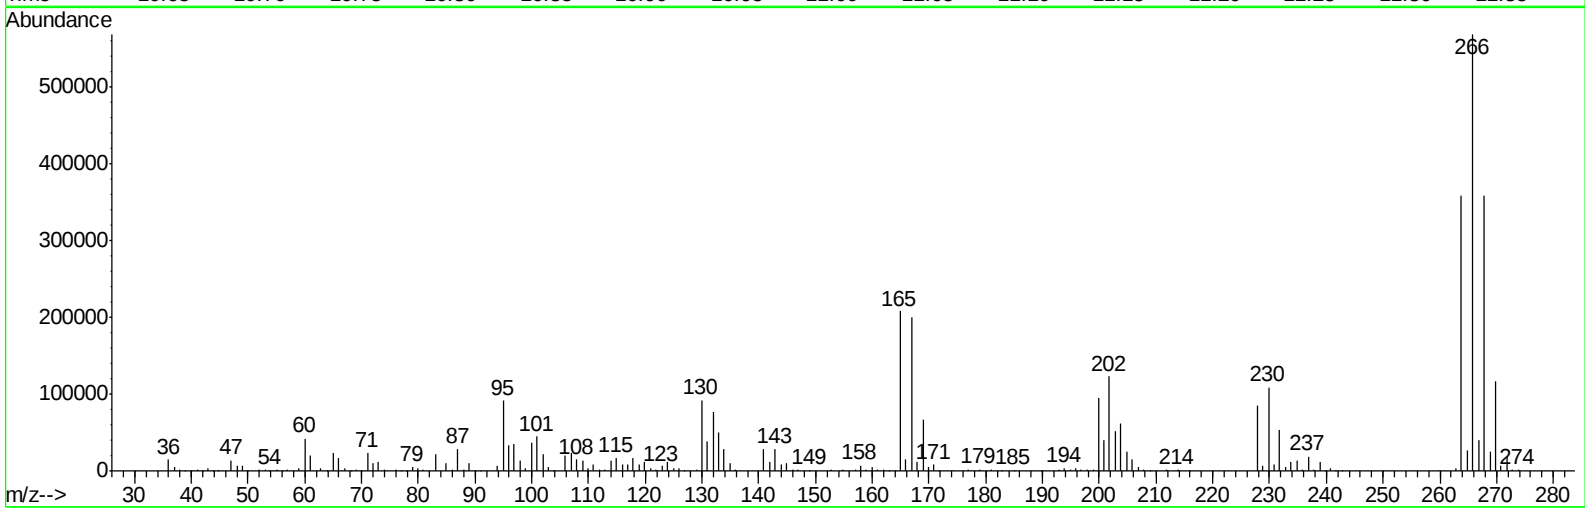


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062719\
Data File : BF115226.D
Acq On : 27 Jun 2019 7:08
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:46:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

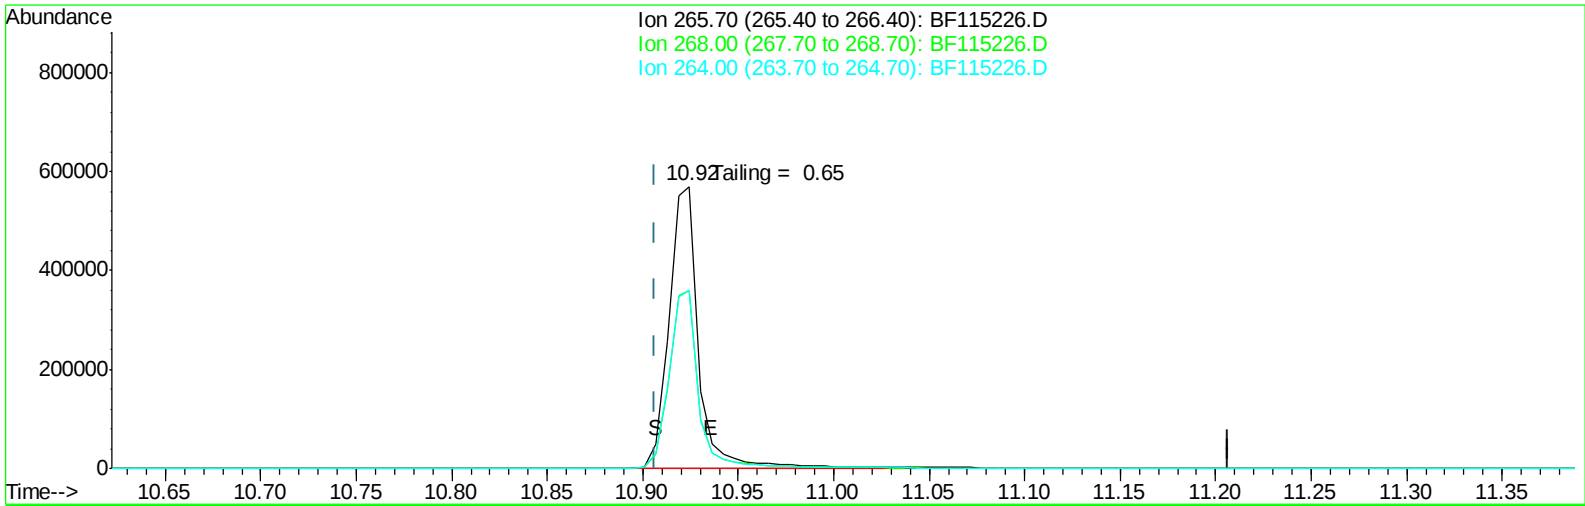

TIC: BF115226.D

(70) Pentachlorophenol (C)

10.924min (+0.018) 107399.71ng

response 631283

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.06
264.00	61.60	62.99
0.00	0.00	0.00