

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062719\
 Data File : BF115231.D
 Acq On : 27 Jun 2019 12:53
 Operator : HP/JU
 Sample : PB120902BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120902BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	549	555	558	rBV	4927605	5277163	71.24%	9.498%
2	6.236	725	731	734	rBV	4830206	5463219	73.75%	9.833%
3	6.366	748	753	756	rBV	5745444	5694153	76.87%	10.249%
4	6.595	788	792	795	rBV	1846736	1437130	19.40%	2.587%
5	6.754	814	819	822	rBV	5332732	4656225	62.86%	8.381%
6	7.160	882	888	891	rBV	3328791	3611075	48.75%	6.499%
7	7.878	1005	1010	1013	rBV	2051145	1833086	24.75%	3.299%
8	8.954	1188	1193	1196	rBV	7068570	6958639	93.94%	12.525%
9	9.619	1301	1306	1310	rBV	2407724	2138989	28.87%	3.850%
10	10.401	1434	1439	1443	rBV	4315442	4351909	58.75%	7.833%
11	11.089	1552	1556	1560	rBV	2623394	2255661	30.45%	4.060%
12	12.677	1821	1826	1829	rBV	6879238	7407843	100.00%	13.333%
13	13.707	1997	2001	2005	rBV	2300096	2069029	27.93%	3.724%
14	15.083	2230	2235	2245	rVB	1897972	2126757	28.71%	3.828%
15	15.977	2383	2387	2393	rVB2	58696	86237	1.16%	0.155%
16	16.489	2469	2474	2482	rVB2	49968	102010	1.38%	0.184%
17	17.089	2569	2576	2582	rBV3	40047	90680	1.22%	0.163%


Sum of corrected areas: 55559805

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062719\
Data File : BF115231.D
Acq On : 27 Jun 2019 12:53
Operator : HP/JU
Sample : PB120902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120902BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

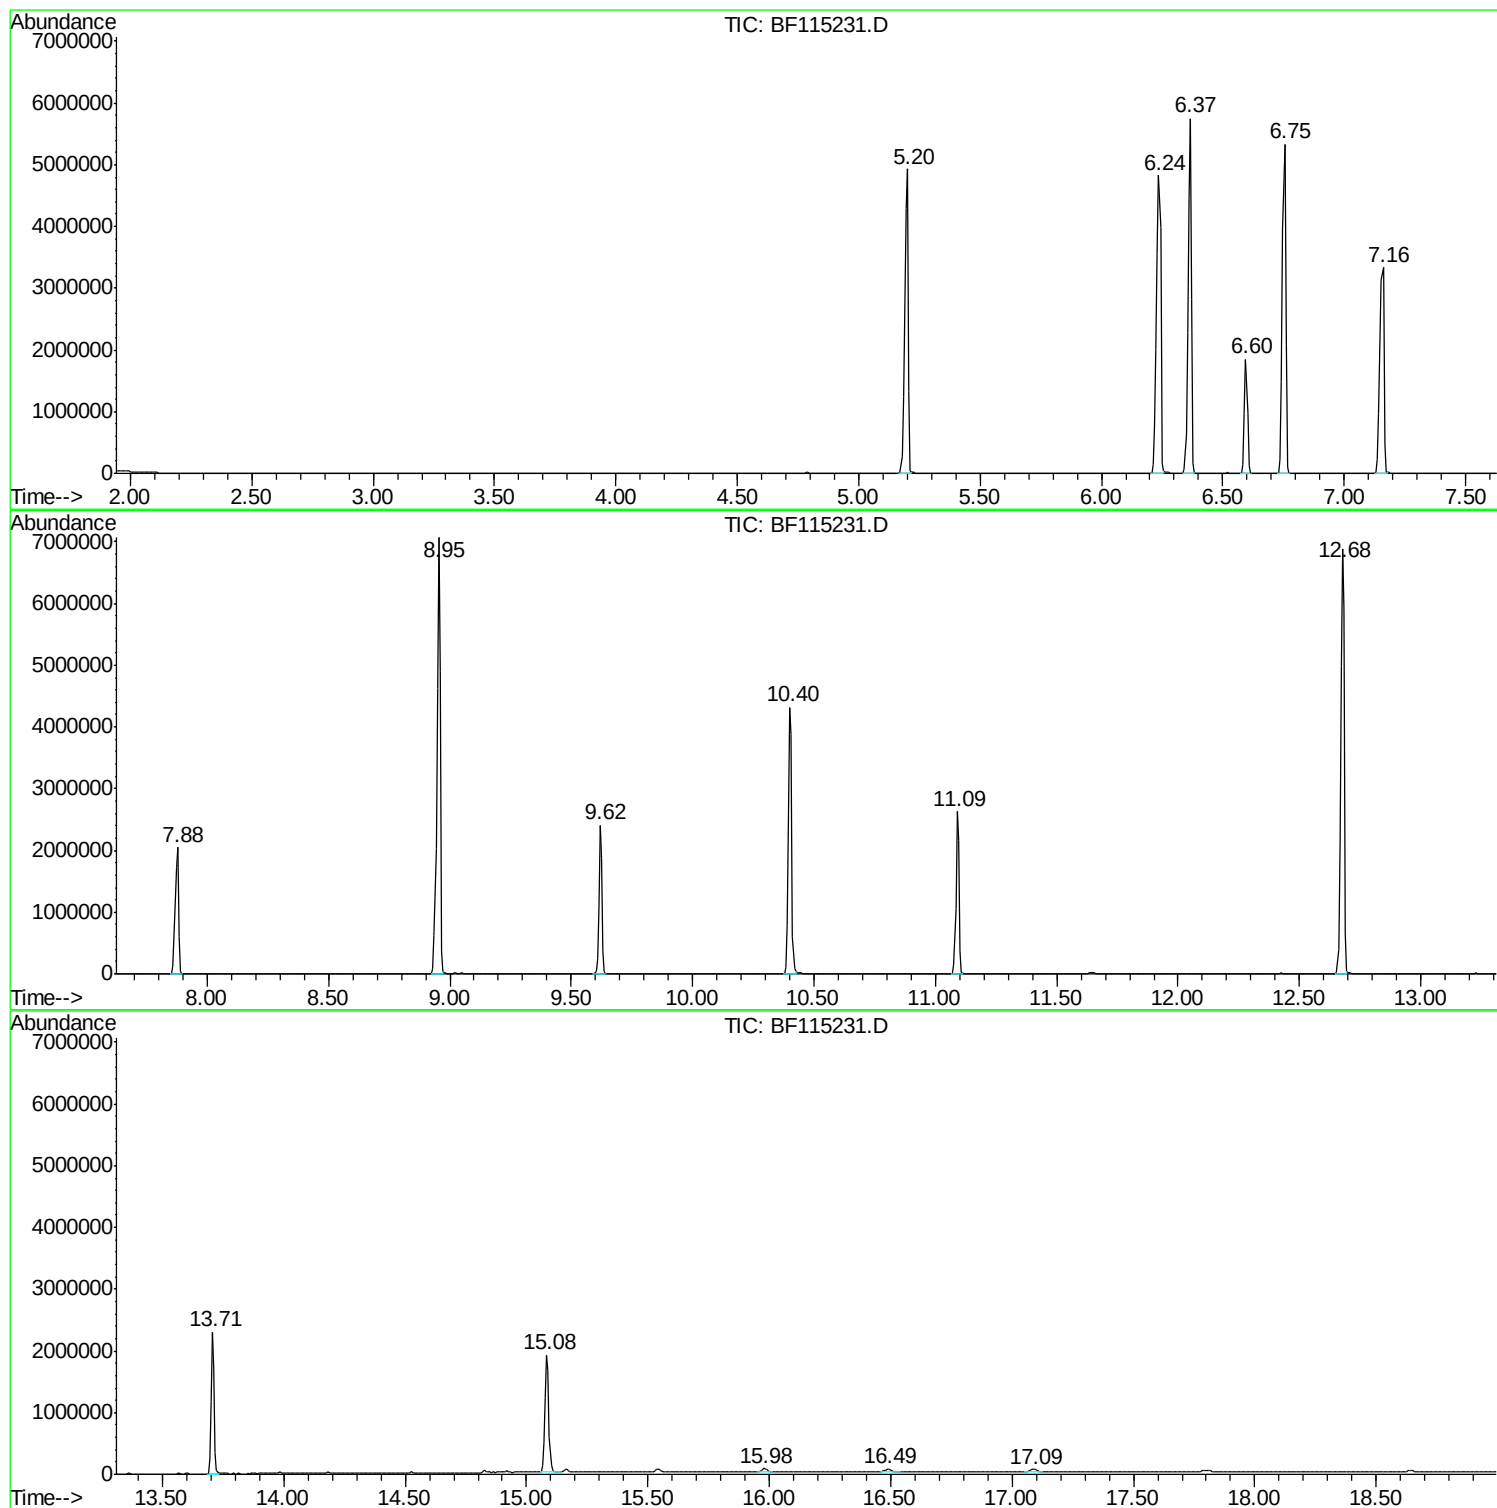

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062719\
Data File : BF115231.D
Acq On : 27 Jun 2019 12:53
Operator : HP/JU
Sample : PB120902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120902BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	79.24 ng	5694150	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	16
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

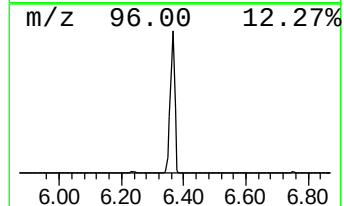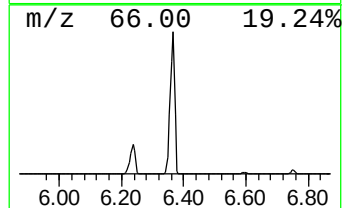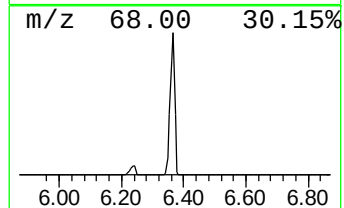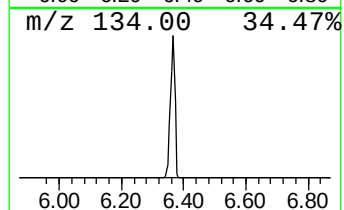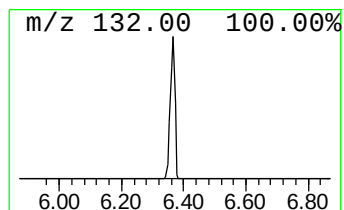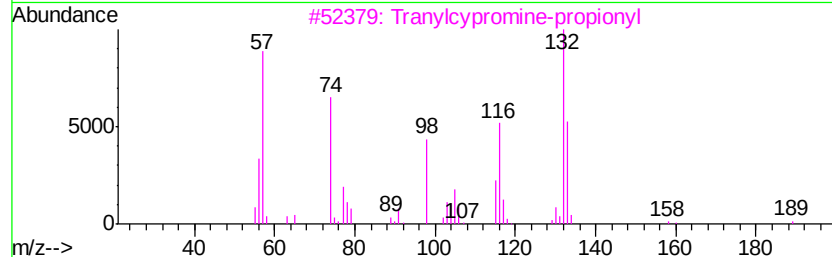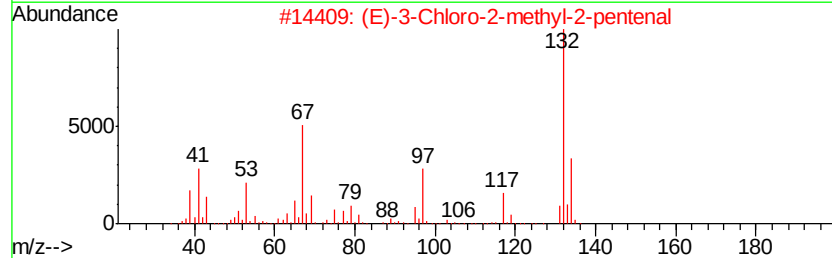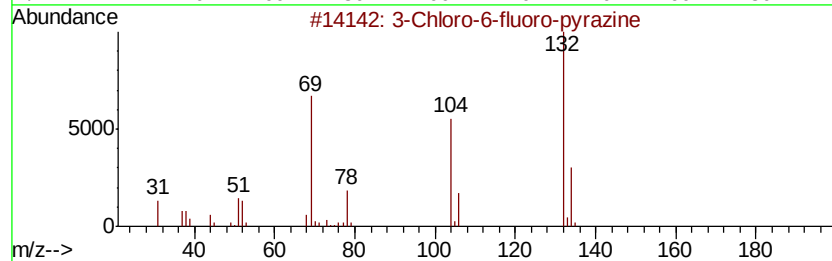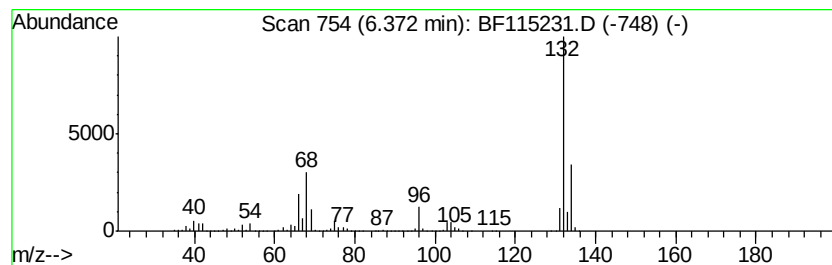

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062719\
Data File : BF115231.D
Acq On : 27 Jun 2019 12:53
Operator : HP/JU
Sample : PB120902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120902BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.37	6.37	79.2	ng	5694150	1	6.60	1437130	20.0