


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF062719\  
 Data File : BF115226.D  
 Acq On : 27 Jun 2019 7:08  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF062119.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jun 28 05:26:43 2019

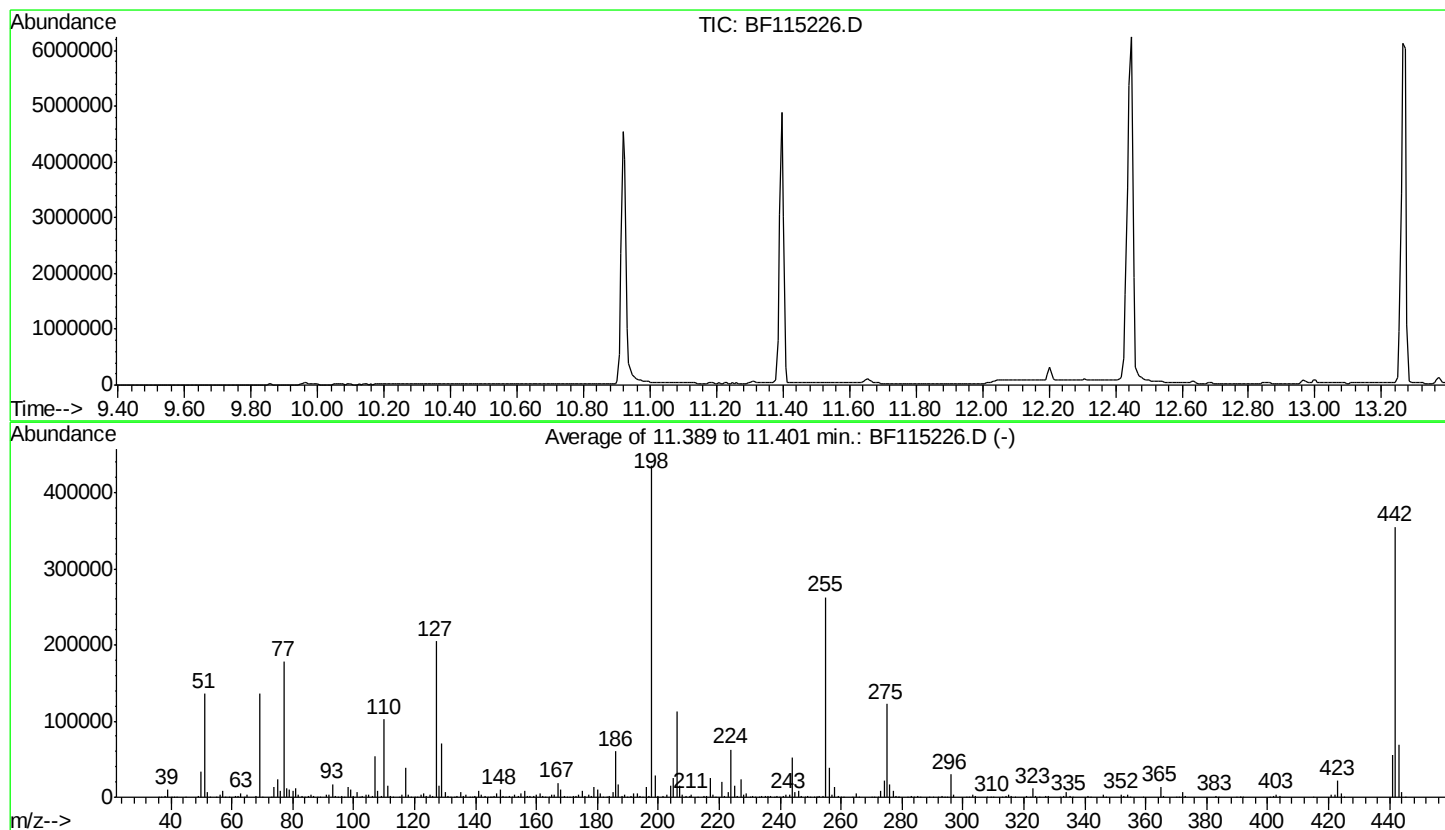

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.2      | 135928  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 2483    | PASS             |
| 69          | 198          | 0.00         | 100          | 31.4      | 136534  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 459     | PASS             |
| 127         | 198          | 10           | 80           | 47.0      | 204714  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 2442    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 435498  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 28842   | PASS             |
| 275         | 198          | 10           | 60           | 28.0      | 122029  | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 14152   | PASS             |
| 441         | 198          | 0.01         | 100          | 12.7      | 55170   | PASS             |
| 442         | 198          | 50           | 100          | 81.5      | 354837  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 68666   | PASS             |