


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062719\
 Data File : BF115240.D
 Acq On : 27 Jun 2019 18:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

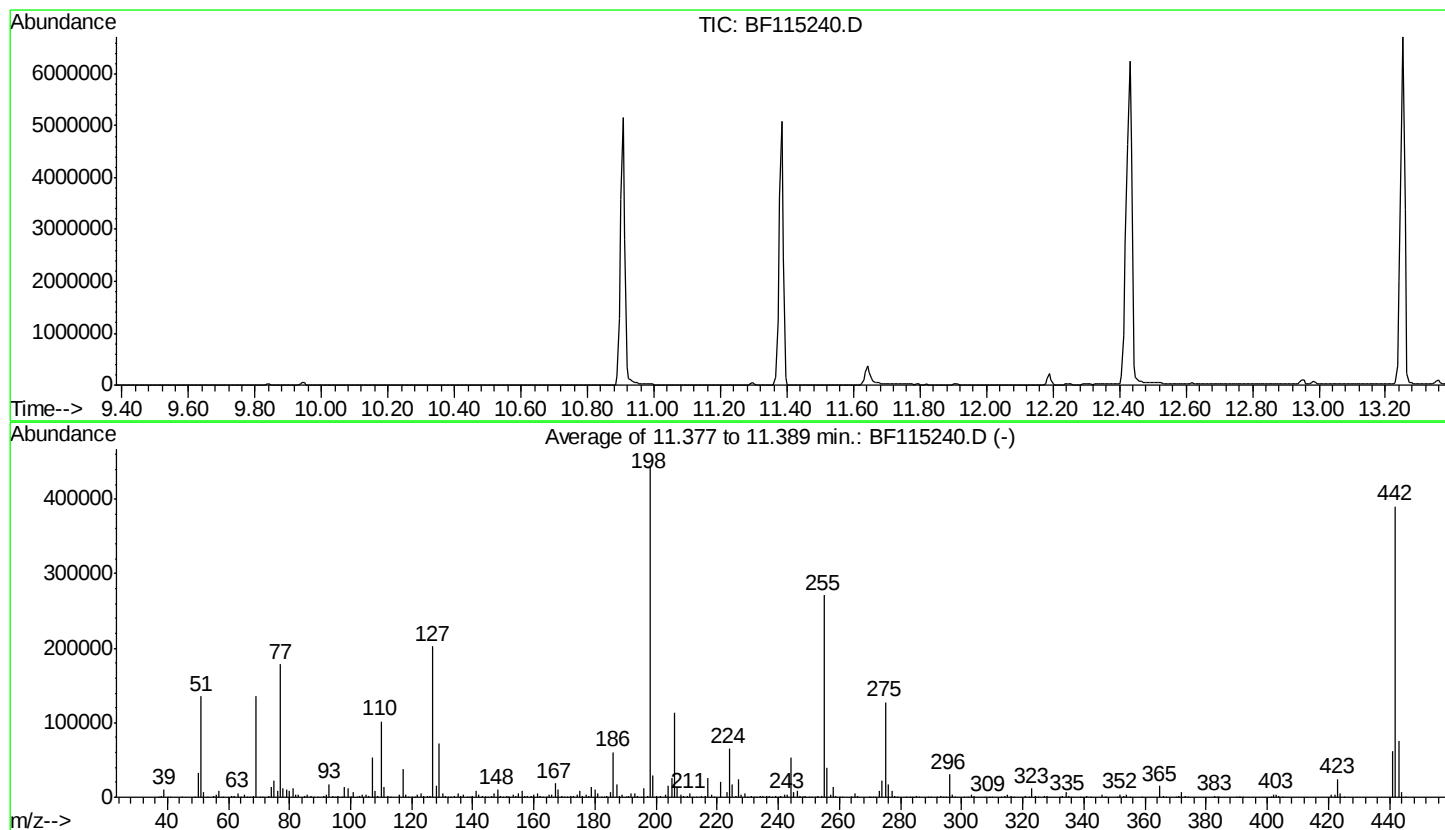

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	135152	PASS
68	69	0.00	2	1.6	2178	PASS
69	198	0.00	100	30.7	136418	PASS
70	69	0.00	2	0.7	897	PASS
127	198	10	80	45.5	202512	PASS
197	198	0.00	2	0.4	1822	PASS
198	198	100	100	100.0	445056	PASS
199	198	5	9	6.7	29674	PASS
275	198	10	60	28.7	127578	PASS
365	198	1	100	3.4	14924	PASS
441	198	0.01	100	13.9	62080	PASS
442	198	50	100	87.6	390037	PASS
443	442	15	24	19.2	74885	PASS