
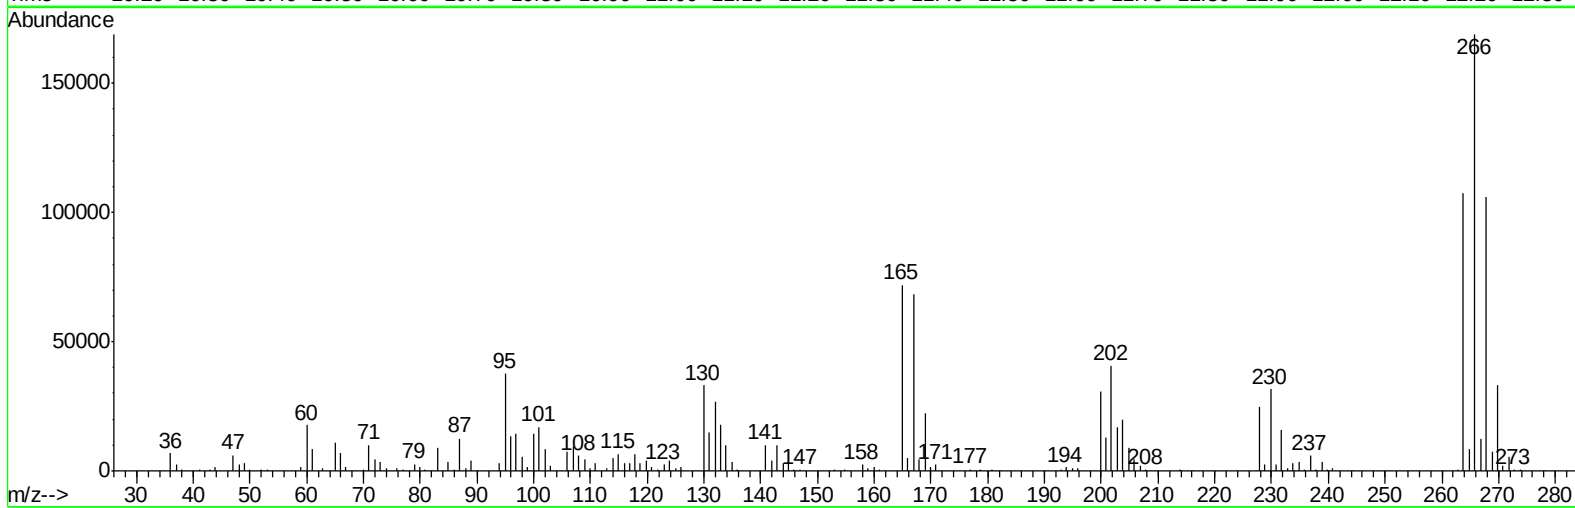


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071219\
Data File : BF115517.D
Acq On : 12 Jul 2019 9:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 05:09:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

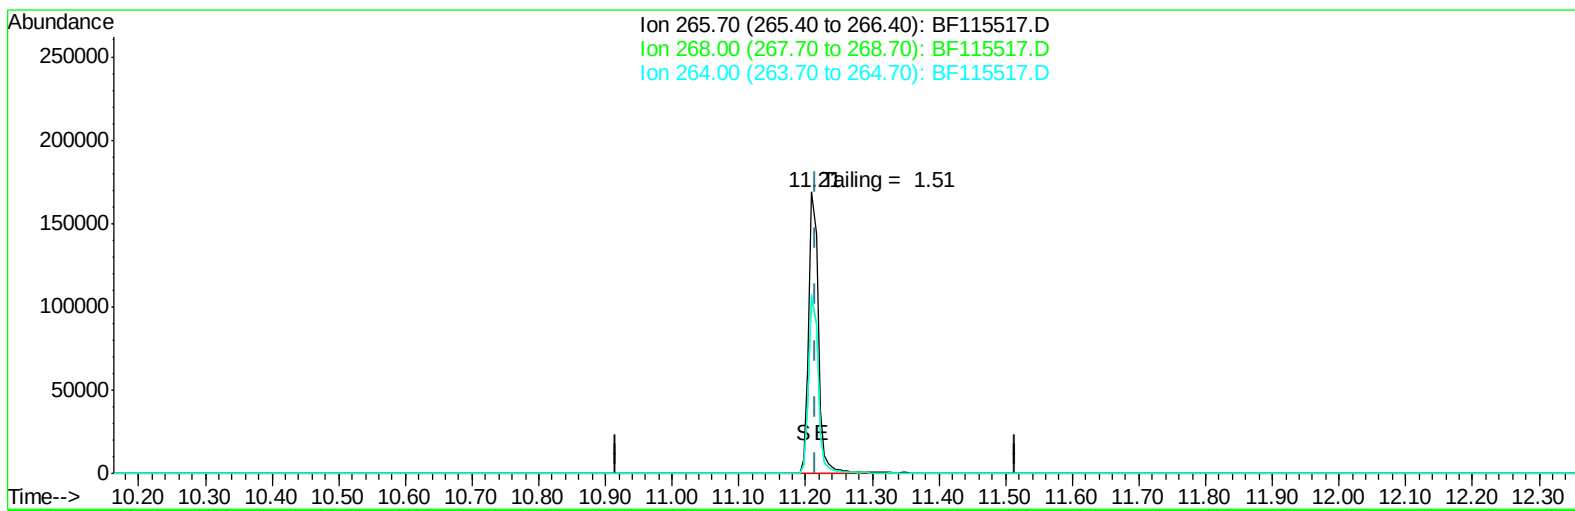

TIC: BF115517.D

(70) Pentachlorophenol (C)



11.210min (-0.006) 35507.82ng

response 162116

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.65
264.00	63.30	63.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071219\
Data File : BF115517.D
Acq On : 12 Jul 2019 9:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 05:09:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

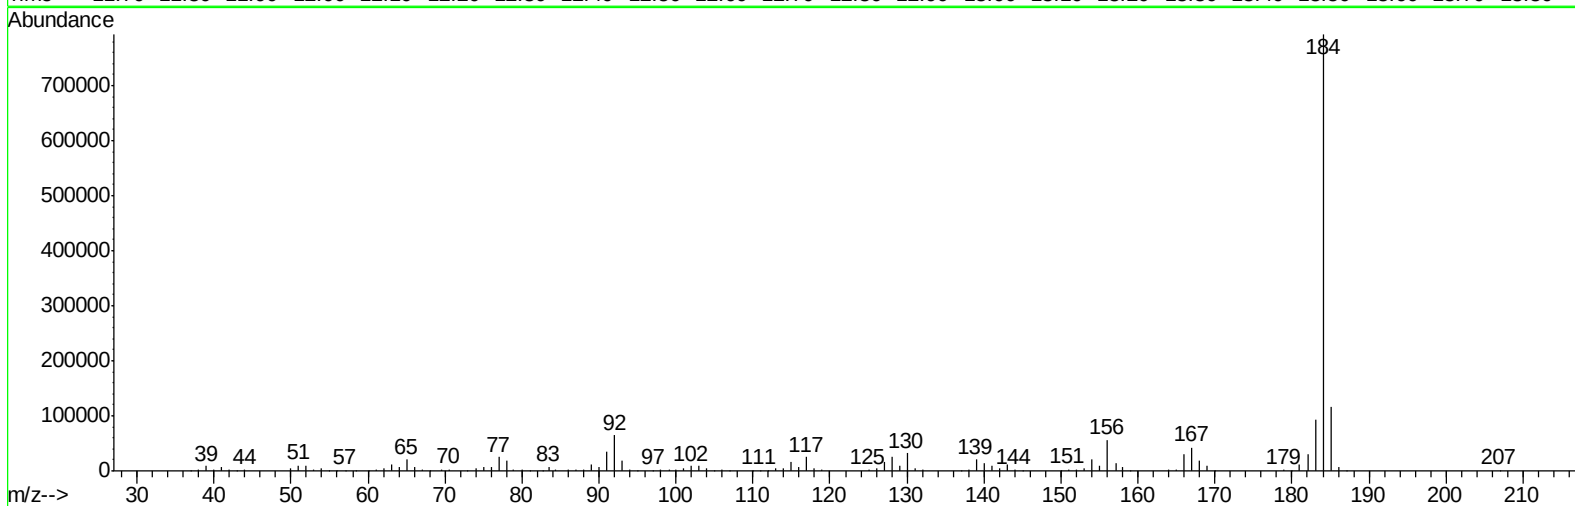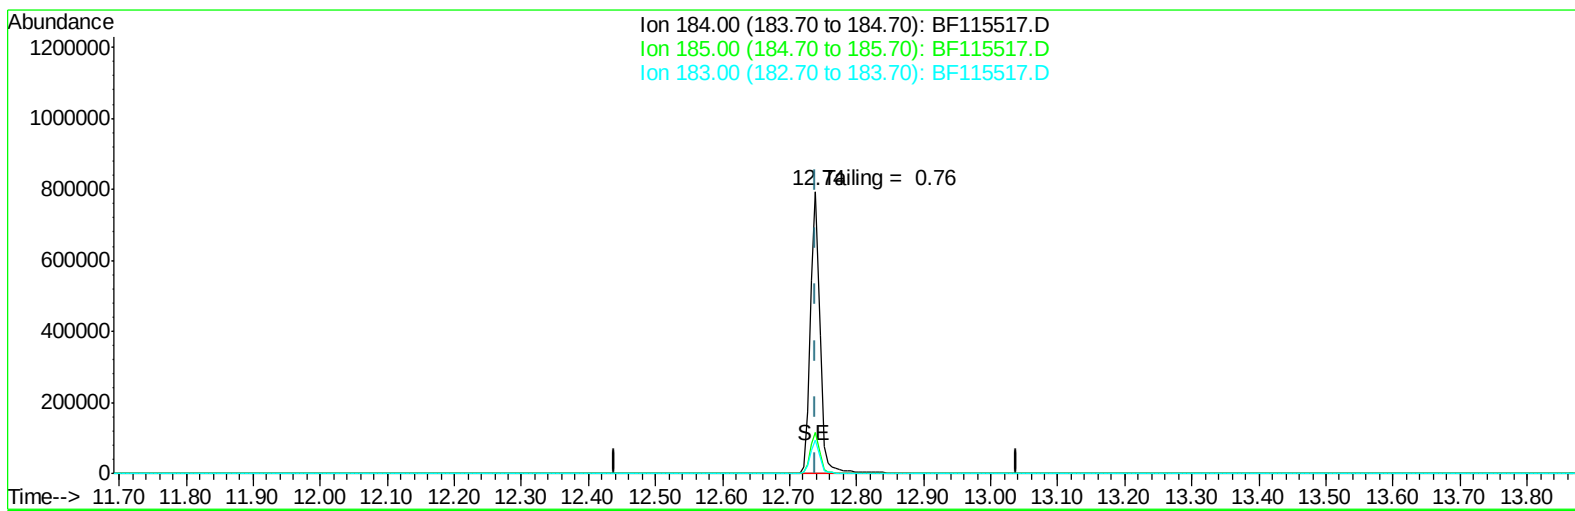

TIC: BF115517.D

(77) Benzidine

12.739min (-0.000) 0.00ng

response 748140

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.71
183.00	11.60	11.76
0.00	0.00	0.00