


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071219\
 Data File : BF115517.D
 Acq On : 12 Jul 2019 9:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

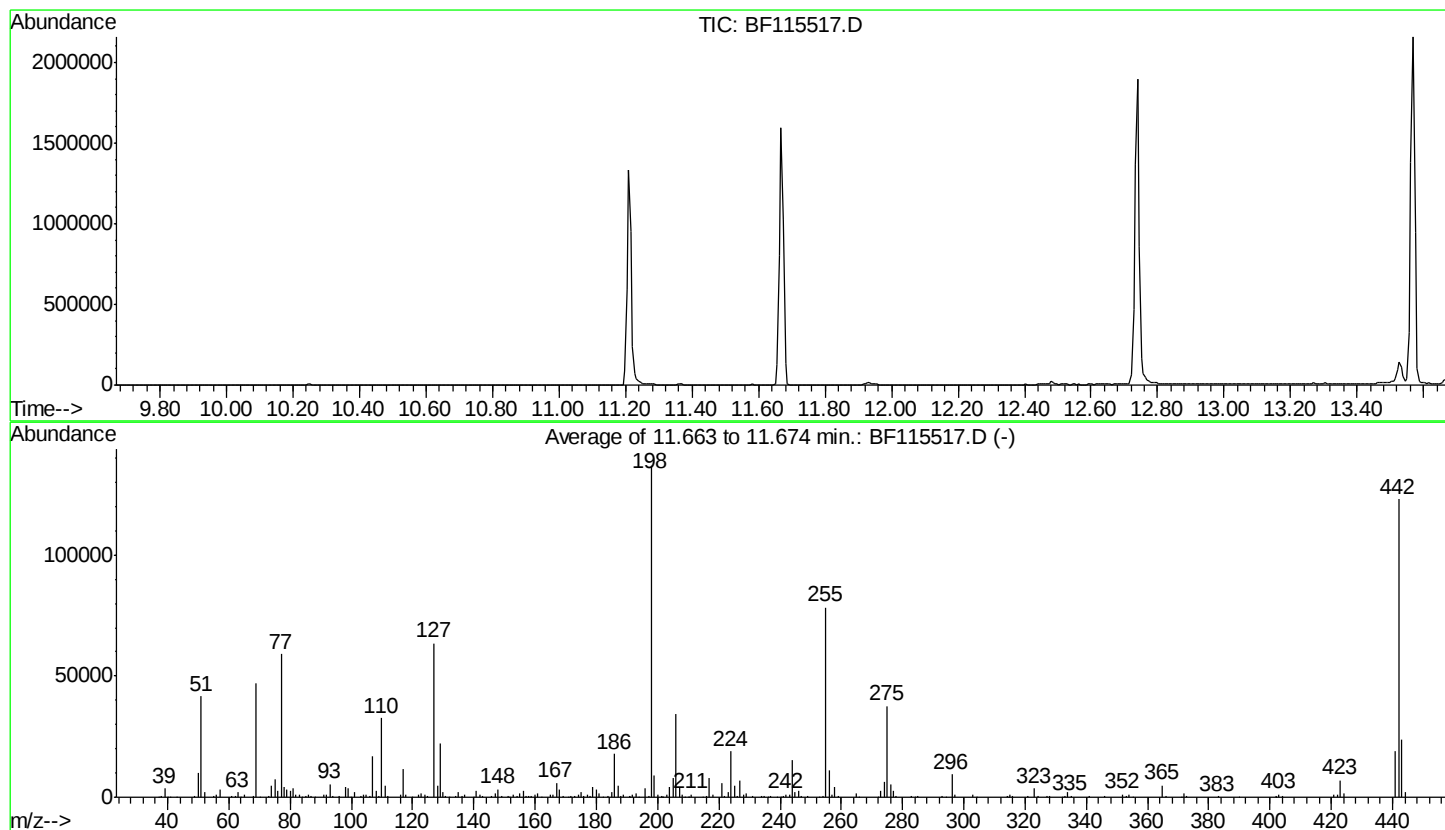

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	41688	PASS
68	69	0.00	2	1.7	775	PASS
69	198	0.00	100	34.2	46792	PASS
70	69	0.00	2	0.2	104	PASS
127	198	10	80	46.4	63544	PASS
197	198	0.00	2	0.6	798	PASS
198	198	100	100	100.0	136837	PASS
199	198	5	9	6.8	9242	PASS
275	198	10	60	27.5	37632	PASS
365	198	1	100	3.5	4776	PASS
441	198	0.01	100	13.9	18986	PASS
442	198	50	100	89.9	123002	PASS
443	442	15	24	19.4	23804	PASS