
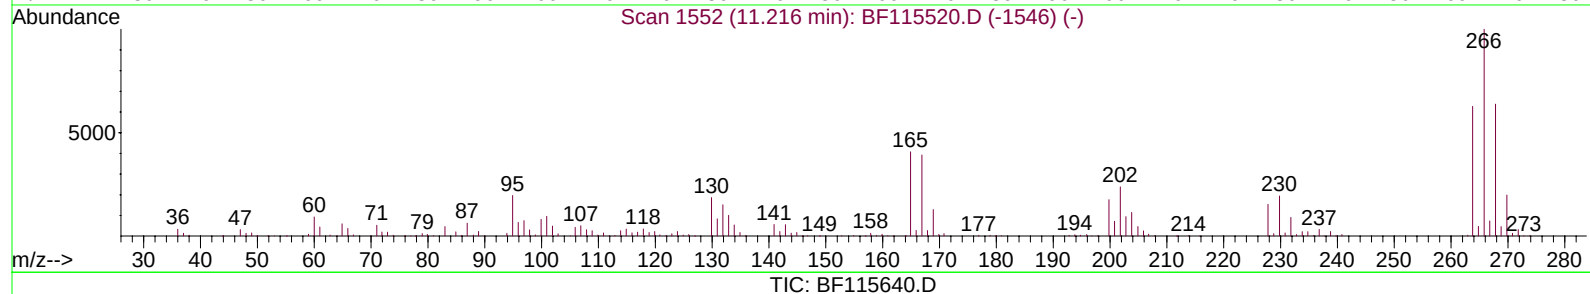
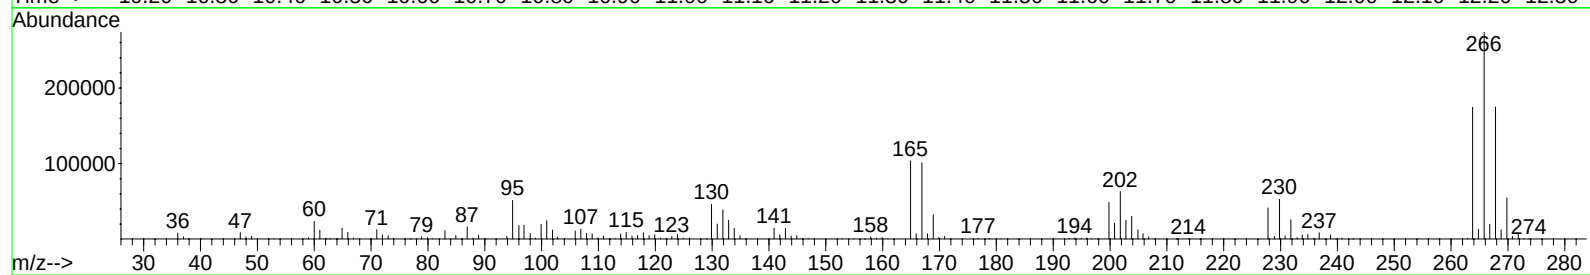


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071819\
Data File : BF115640.D
Acq On : 18 Jul 2019 8:02
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 16:50:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

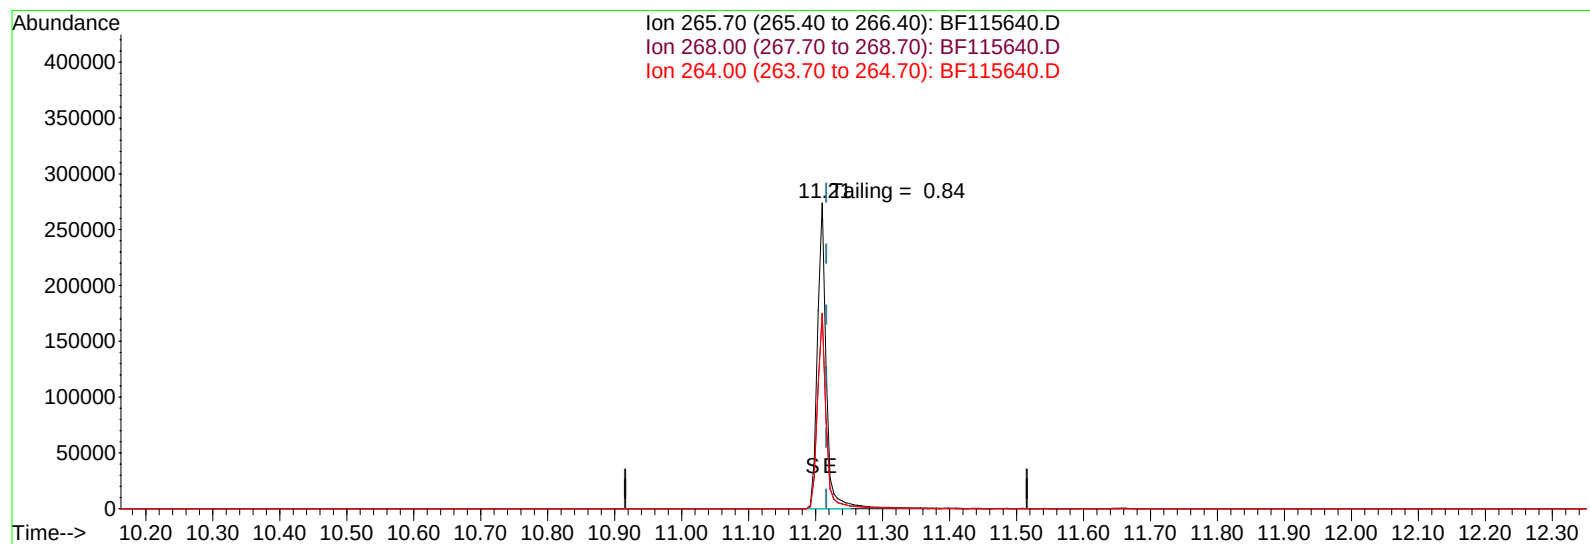

(70) Pentachlorophenol (C)




11.210min (-0.006) 35398.42ng

response 252879

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.87
264.00	63.30	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071819\
 Data File : BF115640.D
 Acq On : 18 Jul 2019 8:02
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 16:50:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 14:03:52 2019
 Response via : Initial Calibration

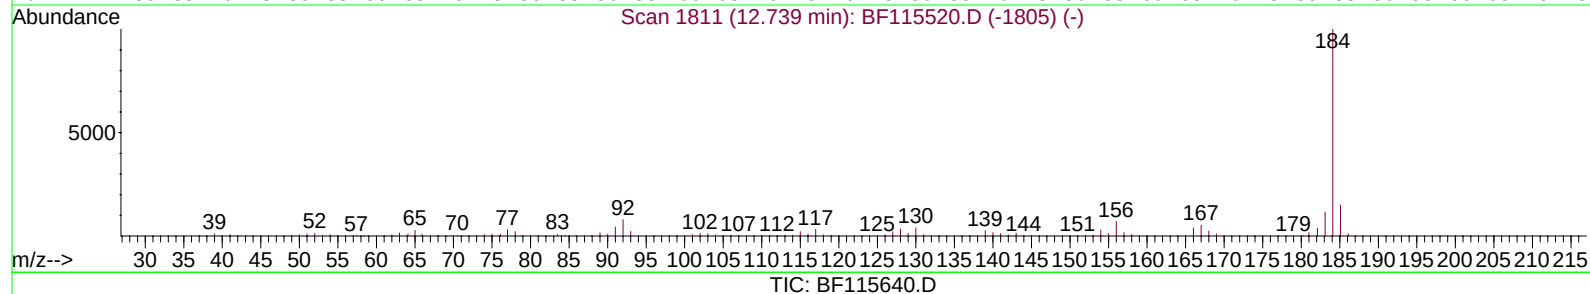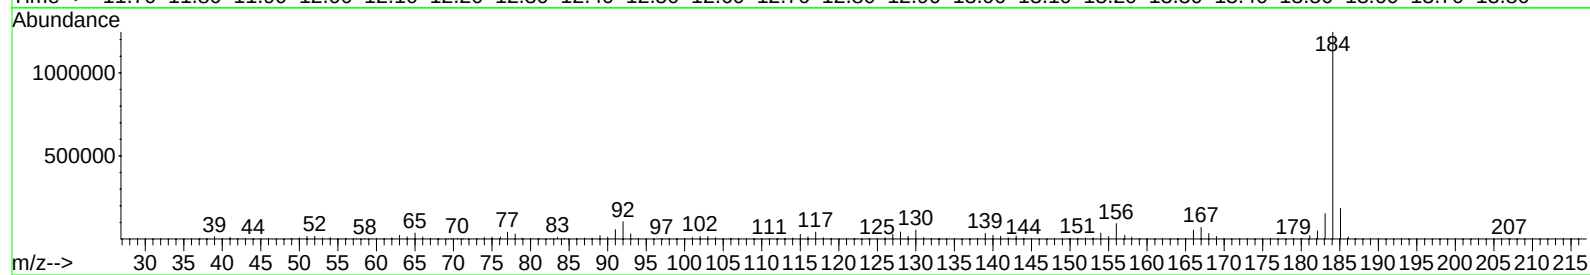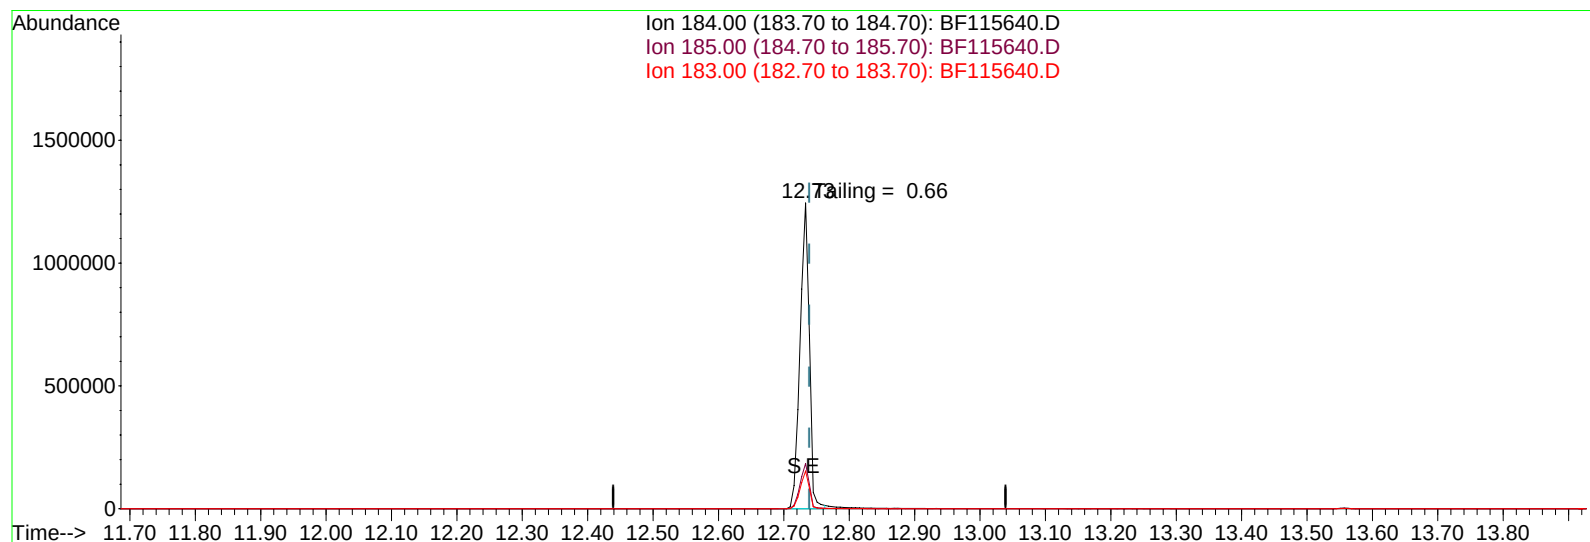

(77) Benzidine

12.733min (-0.006) 0.00ng

response 1256431

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.82
183.00	11.60	12.35
0.00	0.00	0.00