
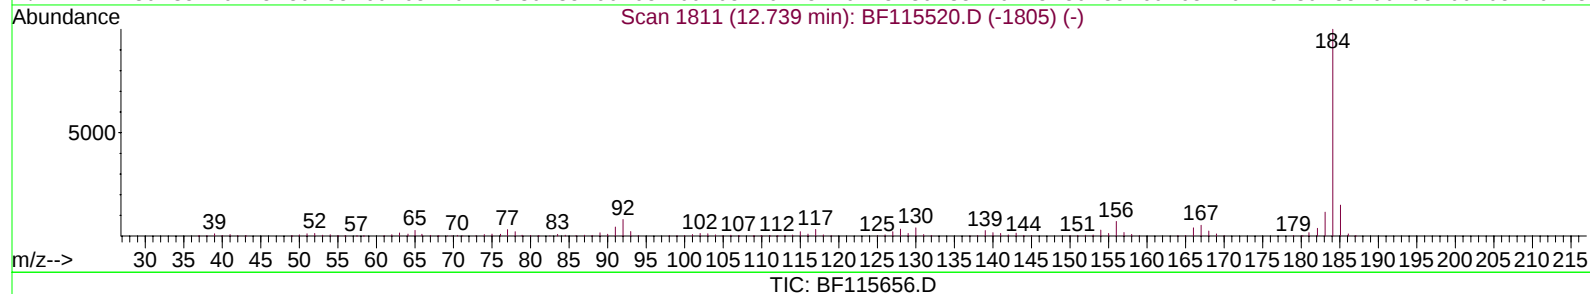
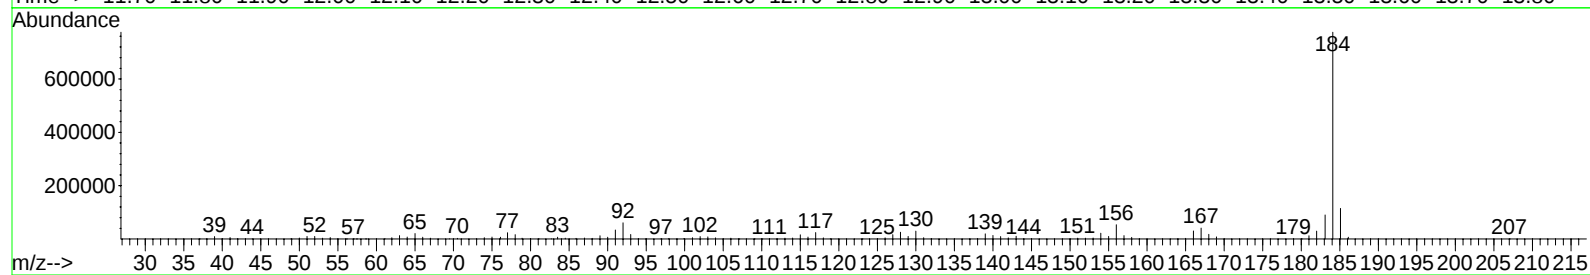


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071819\
Data File : BF115656.D
Acq On : 18 Jul 2019 20:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:32:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

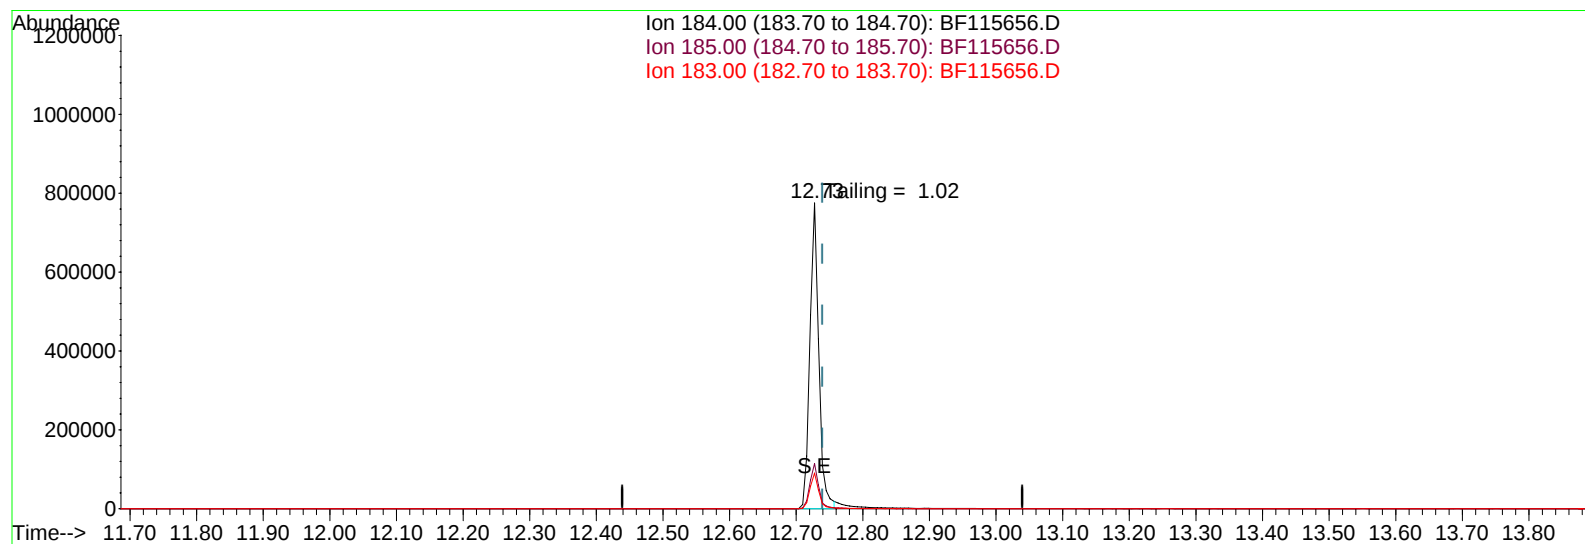

(77) Benzidine




12.727min (-0.012) 0.00ng

response 751559

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.79
183.00	11.60	11.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF071819\
Data File : BF115656.D
Acq On : 18 Jul 2019 20:32
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:32:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

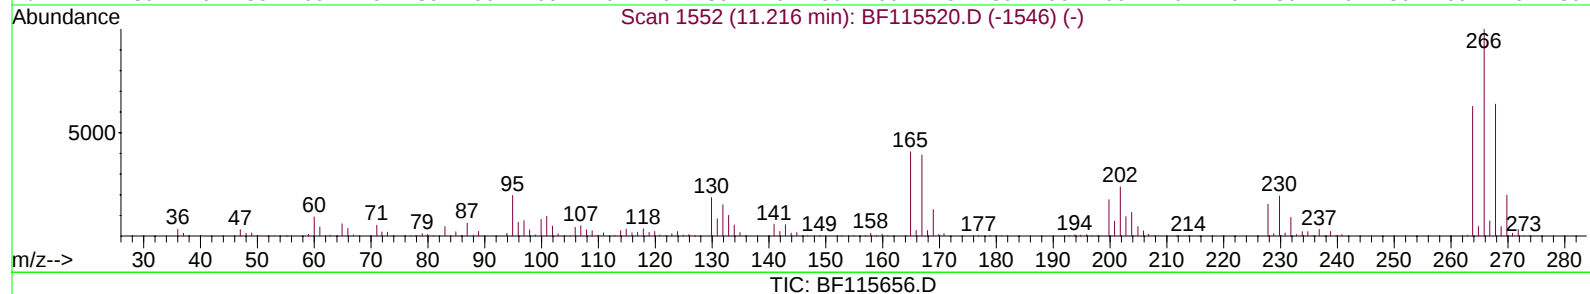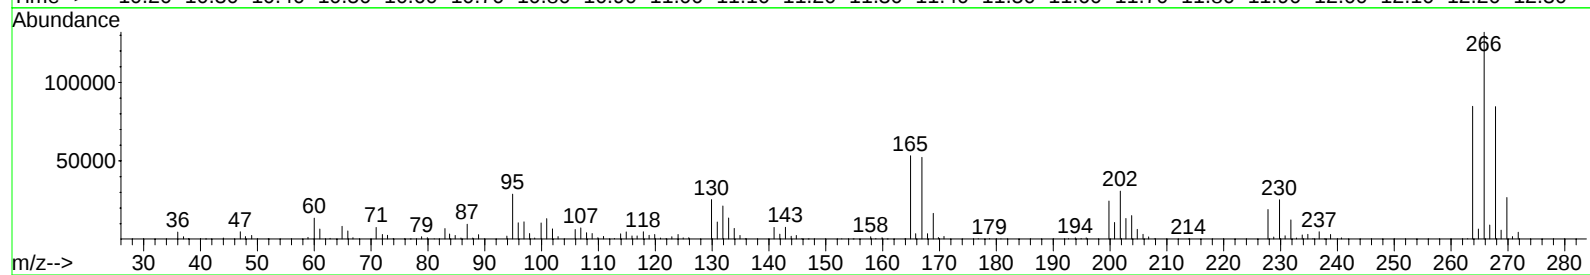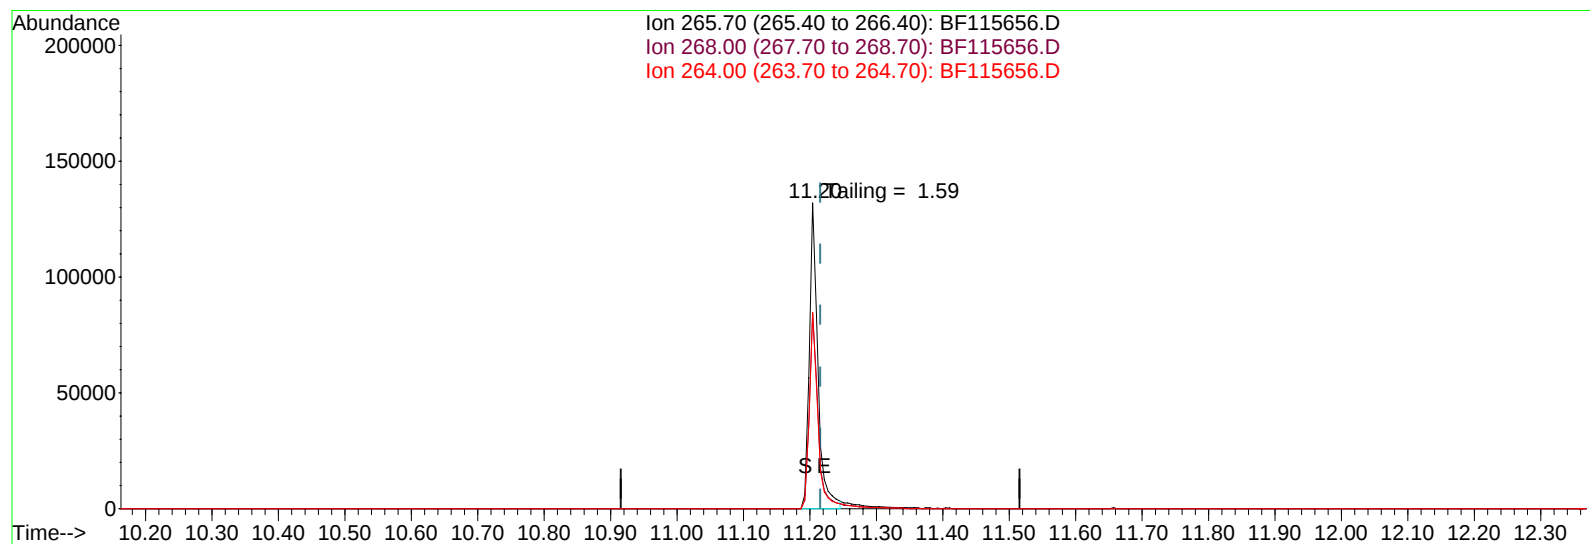

(70) Pentachlorophenol (C)

11.204min (-0.012) 33178.13ng

response 126586

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.12
264.00	63.30	64.23
0.00	0.00	0.00