

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
 Data File : BF115655.D
 Acq On : 18 Jul 2019 18:45
 Operator : HP/JU
 Sample : K3615-05 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-071719-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	6	10	15	rVB	210030	280585	19.27%	1.393%
2	5.498	572	580	593	rBV	1117478	1042140	71.58%	5.174%
3	5.728	613	619	629	rBV4	25583	51180	3.52%	0.254%
4	6.145	687	690	696	rBV4	15269	21311	1.46%	0.106%
5	6.416	734	736	739	rBV2	23166	27768	1.91%	0.138%
6	6.504	744	751	759	rBV	1260932	1126934	77.41%	5.595%
7	6.563	759	761	765	rVB2	34950	35949	2.47%	0.178%
8	6.651	772	776	781	rVB	1398545	1165785	80.08%	5.788%
9	6.716	784	787	788	rBV2	60943	68709	4.72%	0.341%
10	6.887	812	816	819	rBV	1039507	950793	65.31%	4.721%
11	6.945	823	826	830	rVB	43179	41684	2.86%	0.207%
12	7.039	838	842	845	rBV	1143036	916175	62.93%	4.549%
13	7.069	845	847	850	rVB2	31488	27386	1.88%	0.136%
14	7.163	861	863	866	rVB	58253	48136	3.31%	0.239%
15	7.204	866	870	872	rBV2	55984	48471	3.33%	0.241%
16	7.281	880	883	886	rVB3	53898	57499	3.95%	0.285%
17	7.439	902	910	913	rBV	758307	753012	51.72%	3.739%
18	7.487	916	918	921	rVB	81246	67066	4.61%	0.333%
19	7.534	921	926	929	rVB5	54132	81932	5.63%	0.407%
20	7.575	929	933	934	rBV2	25902	31363	2.15%	0.156%
21	7.657	942	947	948	rBV3	20643	23904	1.64%	0.119%
22	7.692	948	953	957	rVB2	65971	89508	6.15%	0.444%
23	7.769	962	966	968	rBV3	33835	38538	2.65%	0.191%
24	7.816	971	974	977	rVV3	52922	60509	4.16%	0.300%
25	7.857	979	981	983	rVB2	27697	20420	1.40%	0.101%
26	7.886	983	986	987	rBV2	61001	53734	3.69%	0.267%
27	7.904	987	989	993	rVV3	87901	99271	6.82%	0.493%
28	7.963	996	999	1001	rVV2	24579	28424	1.95%	0.141%
29	8.004	1004	1006	1009	rVB2	68768	58268	4.00%	0.289%
30	8.034	1009	1011	1016	rBV2	27716	32427	2.23%	0.161%
31	8.075	1016	1018	1021	rVV2	23744	22044	1.51%	0.109%
32	8.122	1021	1026	1028	rVV5	30721	51604	3.54%	0.256%
33	8.163	1028	1033	1040	rVV	1351674	1455853	100.00%	7.228%
34	8.228	1040	1044	1047	rVV4	84953	135432	9.30%	0.672%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071819\
 Data File : BF115655.D
 Acq On : 18 Jul 2019 18:45
 Operator : HP/JU
 Sample : K3615-05 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-071719-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.257	1047	1049	1056	rVB6	50711	59850	4.11%	0.297%
36	8.363	1065	1067	1068	rBV	46615	33599	2.31%	0.167%
37	8.410	1071	1075	1078	rBV4	20181	24000	1.65%	0.119%
38	8.457	1078	1083	1086	rBV3	81494	108508	7.45%	0.539%
39	8.516	1090	1093	1095	rVB3	61433	49870	3.43%	0.248%
40	8.551	1095	1099	1102	rBV3	81203	88952	6.11%	0.442%
41	8.586	1102	1105	1107	rBV	58448	52338	3.60%	0.260%
42	8.610	1107	1109	1111	rVB2	49864	34997	2.40%	0.174%
43	8.633	1111	1113	1115	rVB2	61448	44349	3.05%	0.220%
44	8.669	1116	1119	1122	rBV2	157509	137674	9.46%	0.684%
45	8.710	1124	1126	1131	rVB5	36487	35177	2.42%	0.175%
46	8.757	1131	1134	1138	rBV3	158342	163135	11.21%	0.810%
47	8.798	1138	1141	1142	rVV3	33435	35330	2.43%	0.175%
48	8.822	1143	1145	1147	rVV	61666	56984	3.91%	0.283%
49	8.857	1147	1151	1153	rVB4	35301	47166	3.24%	0.234%
50	8.916	1159	1161	1163	rBV2	43468	36502	2.51%	0.181%
51	8.939	1163	1165	1167	rVV3	21357	26163	1.80%	0.130%
52	8.986	1170	1173	1176	rVB3	73249	80386	5.52%	0.399%
53	9.110	1191	1194	1195	rBV2	33731	34183	2.35%	0.170%
54	9.163	1200	1203	1204	rBV	38096	27178	1.87%	0.135%
55	9.186	1204	1207	1212	rBV3	74049	89155	6.12%	0.443%
56	9.233	1212	1215	1221	rVB	1650792	1305558	89.68%	6.482%
57	9.281	1221	1223	1226	rVB4	37076	35291	2.42%	0.175%
58	9.322	1226	1230	1234	rBV	141287	150510	10.34%	0.747%
59	9.386	1239	1241	1244	rVB	56134	51633	3.55%	0.256%
60	9.480	1254	1257	1258	rBV2	23053	23620	1.62%	0.117%
61	9.557	1267	1270	1271	rBV3	35519	36990	2.54%	0.184%
62	9.575	1271	1273	1275	rVV3	62878	58767	4.04%	0.292%
63	9.598	1275	1277	1279	rVV2	88035	80700	5.54%	0.401%
64	9.628	1279	1282	1286	rVV2	169404	222390	15.28%	1.104%
65	9.663	1286	1288	1290	rVV3	54614	48435	3.33%	0.240%
66	9.698	1292	1294	1297	rVB3	53698	43448	2.98%	0.216%
67	9.763	1302	1305	1309	rBV2	39470	43495	2.99%	0.216%
68	9.851	1315	1320	1323	rVB	80240	84225	5.79%	0.418%
69	9.916	1327	1331	1336	rVB	1433075	1206743	82.89%	5.991%
70	10.022	1346	1349	1356	rVB7	26861	35668	2.45%	0.177%
71	10.086	1356	1360	1362	rBV3	22507	34633	2.38%	0.172%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071819\
 Data File : BF115655.D
 Acq On : 18 Jul 2019 18:45
 Operator : HP/JU
 Sample : K3615-05 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-071719-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	10.175	1373	1375	1379	rVB4	30951	33183	2.28%	0.165%
73	10.239	1383	1386	1392	rBV5	23874	41935	2.88%	0.208%
74	10.345	1399	1404	1407	rBV2	65324	67313	4.62%	0.334%
75	10.433	1416	1419	1421	rVB	48565	37957	2.61%	0.188%
76	10.569	1437	1442	1447	rVB4	27959	41234	2.83%	0.205%
77	10.698	1460	1464	1469	rBV	670954	614407	42.20%	3.051%
78	10.822	1482	1485	1493	rVB3	45985	73955	5.08%	0.367%
79	11.204	1547	1550	1554	rVB4	18302	20525	1.41%	0.102%
80	11.269	1558	1561	1563	rVV	38429	39105	2.69%	0.194%
81	11.298	1563	1566	1572	rVB2	39698	43079	2.96%	0.214%
82	11.398	1579	1583	1587	rBV	1305684	1136921	78.09%	5.645%
83	11.457	1590	1593	1598	rVB2	49375	56690	3.89%	0.281%
84	11.692	1630	1633	1637	rVB2	31397	27308	1.88%	0.136%
85	11.922	1666	1672	1676	rBV3	87925	117204	8.05%	0.582%
86	12.098	1699	1702	1705	rVB	31781	24809	1.70%	0.123%
87	12.380	1747	1750	1755	rBV7	17537	29760	2.04%	0.148%
88	12.451	1759	1762	1764	rBV2	20911	23302	1.60%	0.116%
89	12.486	1765	1768	1770	rVB2	41811	35361	2.43%	0.176%
90	12.610	1786	1789	1794	rBV	89766	85628	5.88%	0.425%
91	12.704	1802	1805	1809	rBV3	31959	42657	2.93%	0.212%
92	12.839	1822	1828	1830	rBV2	93090	143457	9.85%	0.712%
93	12.980	1848	1852	1855	rBV	1329844	1126649	77.39%	5.594%
94	13.116	1873	1875	1878	rBV3	30602	26566	1.82%	0.132%
95	13.210	1889	1891	1893	rBV2	36821	32760	2.25%	0.163%
96	13.557	1946	1950	1951	rBV2	157840	191510	13.15%	0.951%
97	14.033	2027	2031	2034	rBV	1188026	1167501	80.19%	5.797%
98	14.198	2057	2059	2064	rVB	109936	97059	6.67%	0.482%
99	14.810	2161	2163	2166	rBV	111542	88041	6.05%	0.437%
100	15.504	2277	2281	2285	rBV	676226	933745	64.14%	4.636%


Sum of corrected areas: 20141037

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

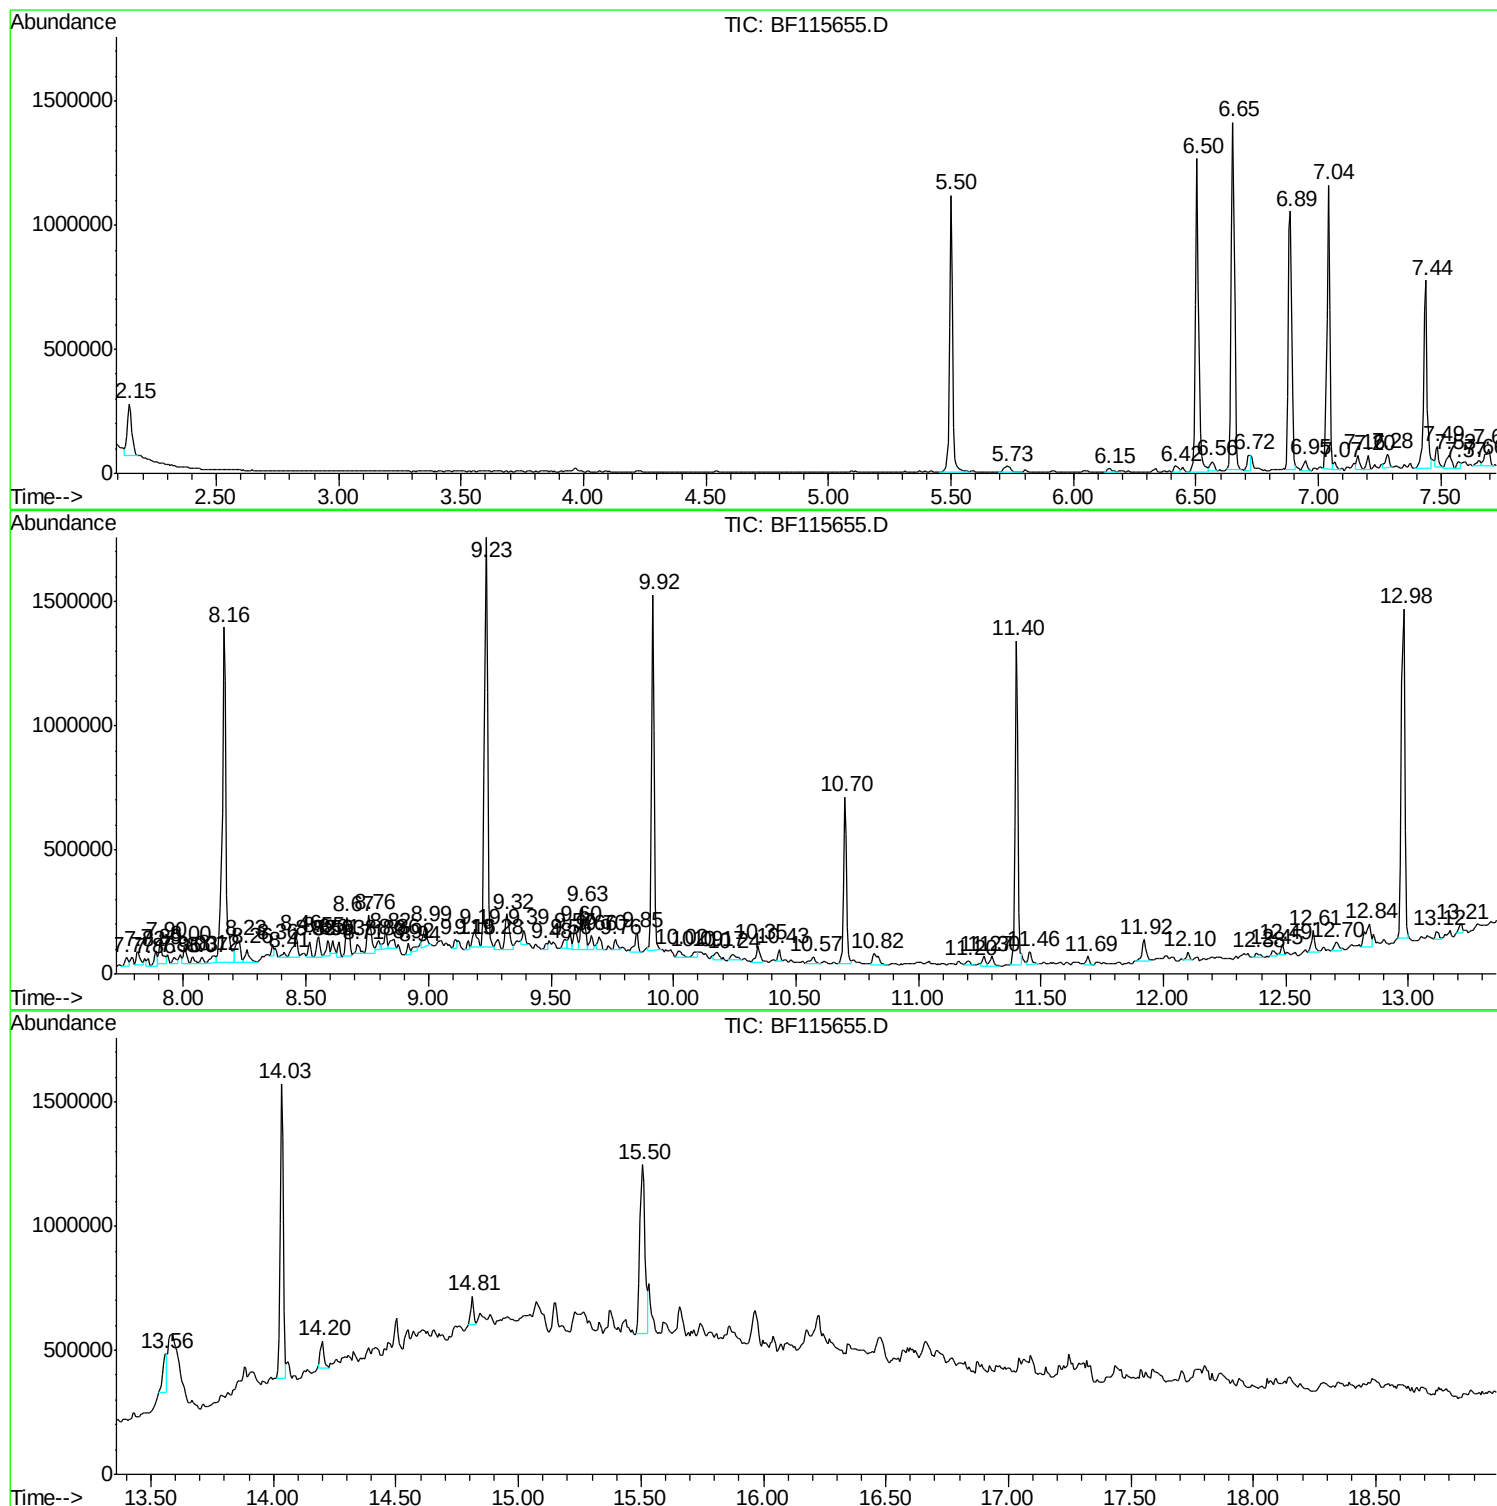

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.15	5.90 ng	280585	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
3		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17
4		Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	10
5		N-Ethylformamide	73	C3H7NO	000627-45-2	9

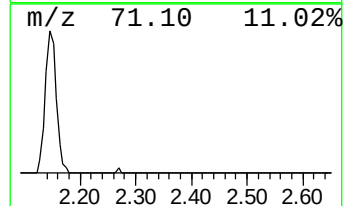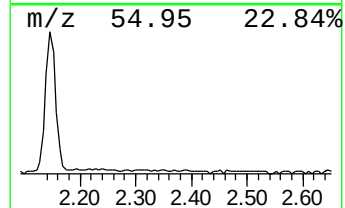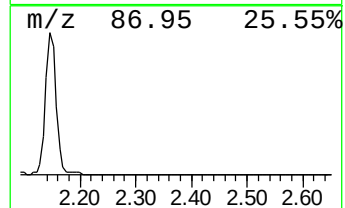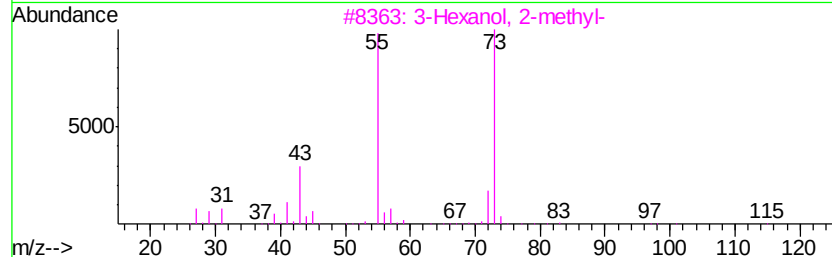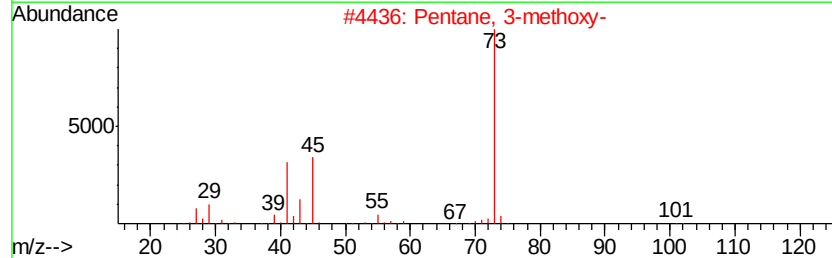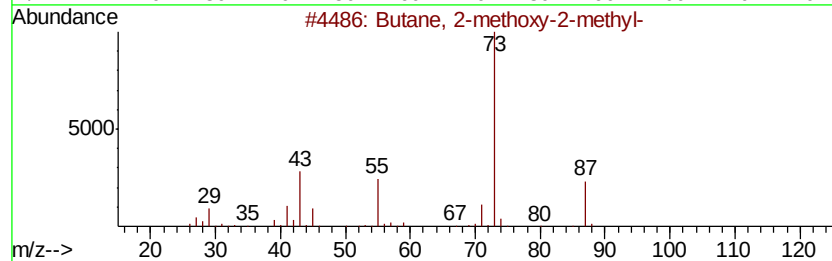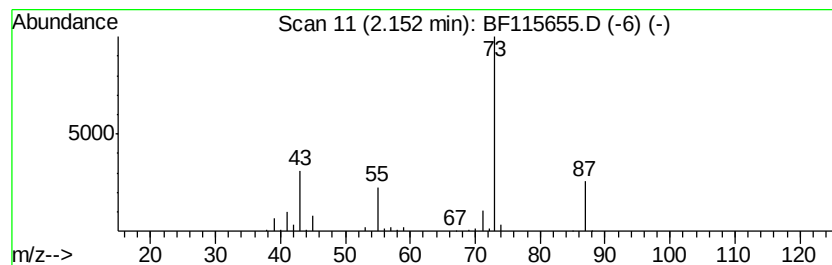

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	24.52 ng	1165790	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

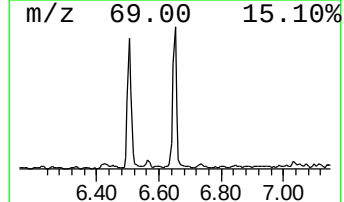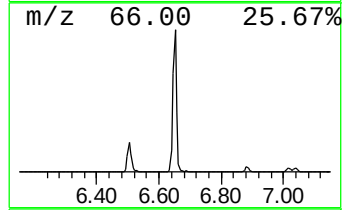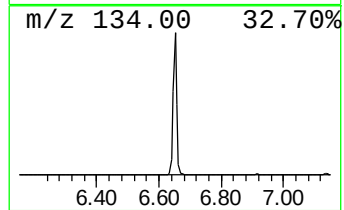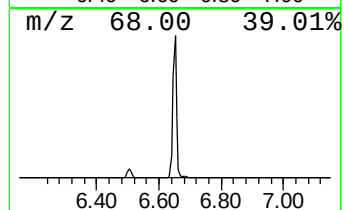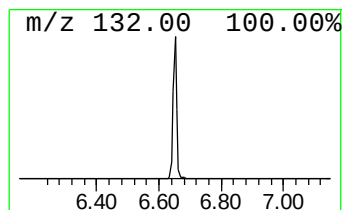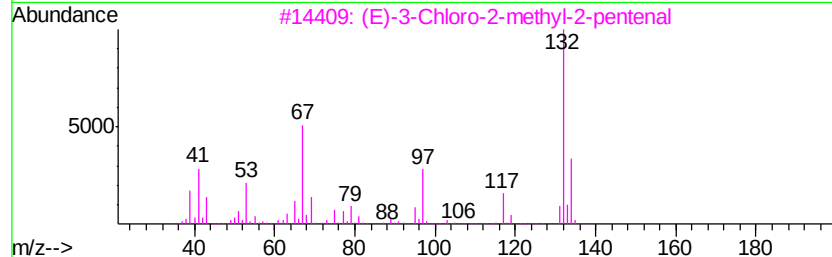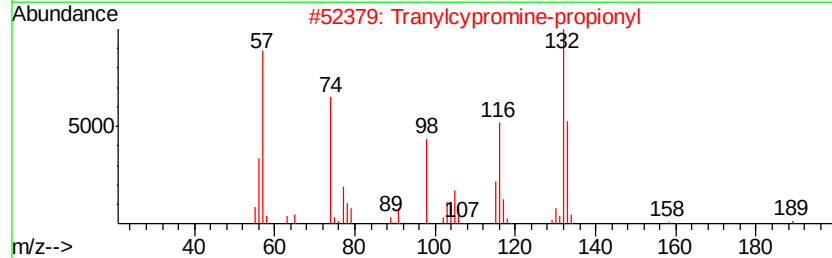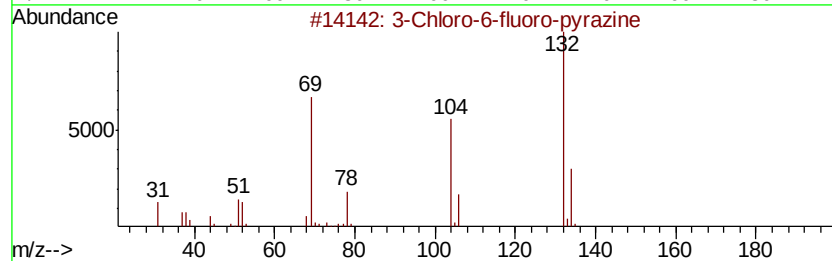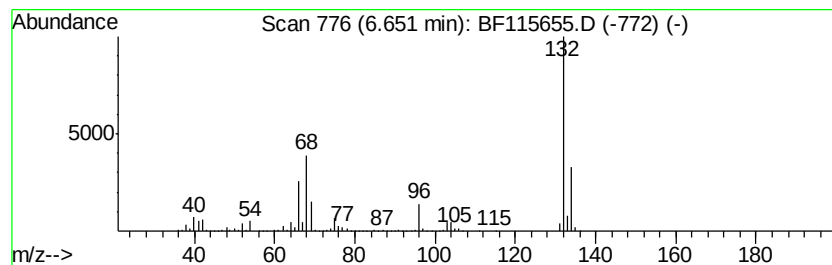

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Tridecane Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.76	2.24 ng	163135	Naphthalene-d8	8.16

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tridecane	184	C13H28	000629-50-5	92
2		Tridecane, 1-iodo-	310	C13H27I	035599-77-0	49
3		Dodecane, 2-methyl-	184	C13H28	001560-97-0	49
4		Dodecane	170	C12H26	000112-40-3	46
5		Pentadecane	212	C15H32	000629-62-9	46

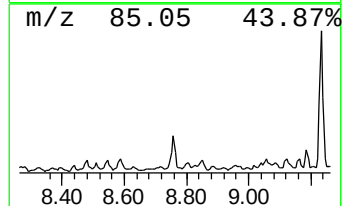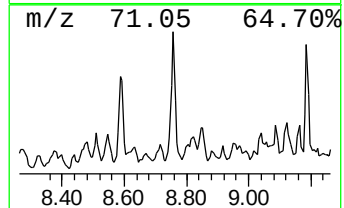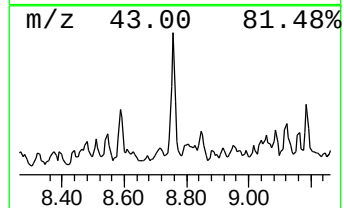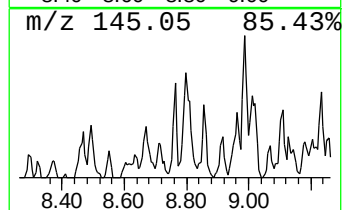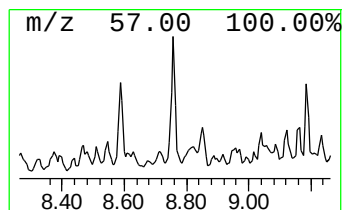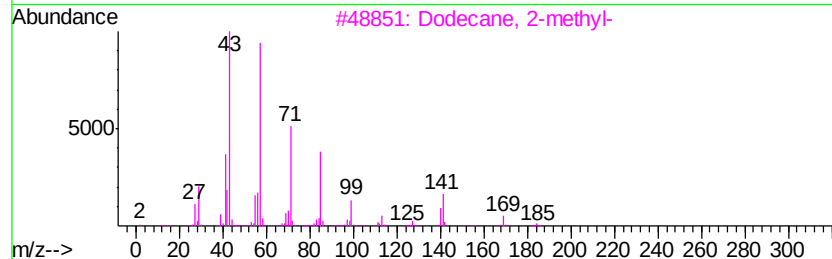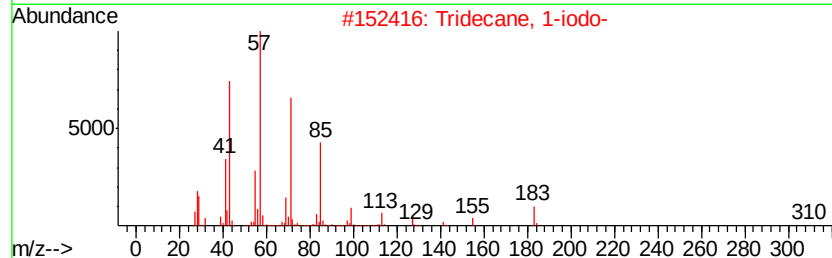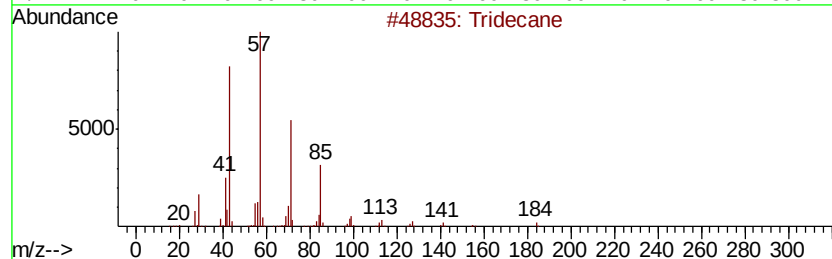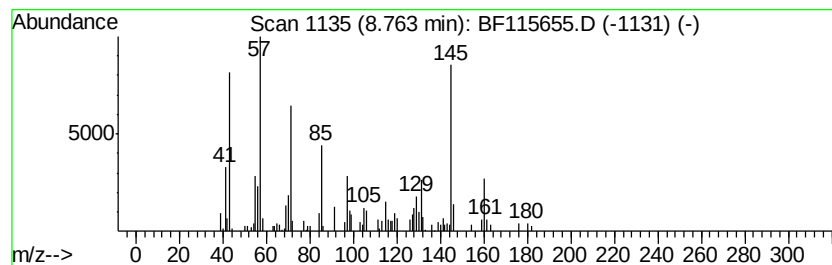

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Nonadecane Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.32	2.49 ng	150510	Acenaphthene-d10	9.92
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Nonadecane	268 C19H40	000629-92-5	87
2	Tetradecane	198 C14H30	000629-59-4	81
3	Tritetracontane	605 C43H88	007098-21-7	80
4	Eicosane, 10-methyl-	296 C21H44	054833-23-7	72
5	Hexane, 2,3,4-trimethyl-	128 C9H20	000921-47-1	64

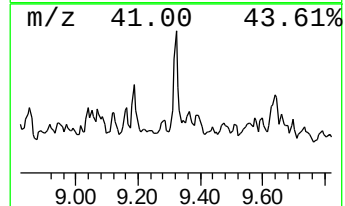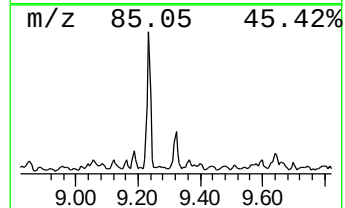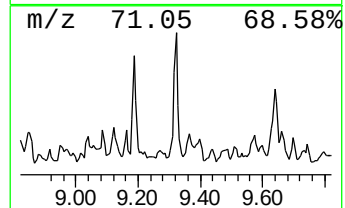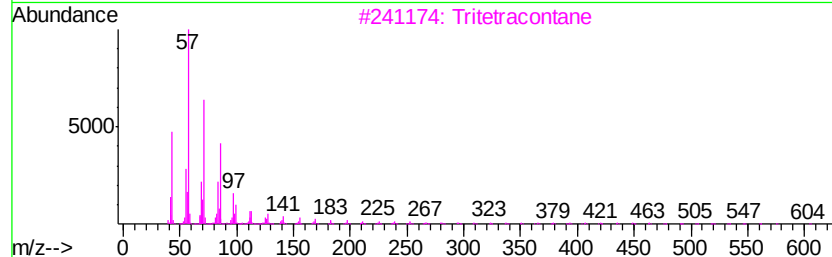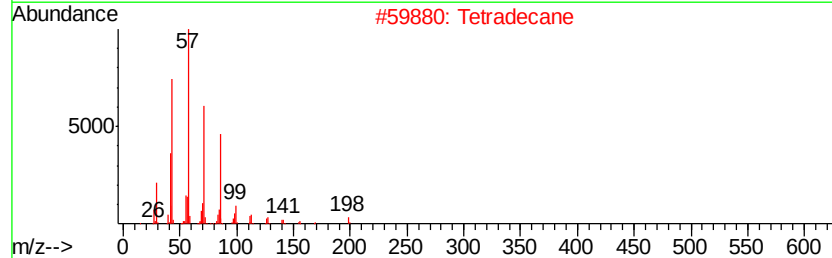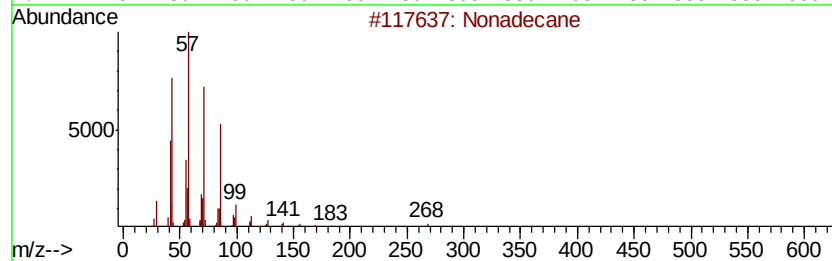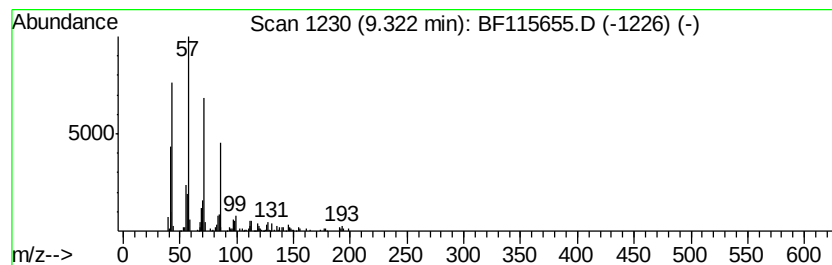

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 n-Hexadecanoic acid Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.92	2.06 ng	117204	Phenanthrene-d10	11.40

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		n-Hexadecanoic acid	256	C16H32O2	000057-10-3	96
2		Pentadecanoic acid	242	C15H30O2	001002-84-2	68
3		Tetradecanoic acid	228	C14H28O2	000544-63-8	64
4		Tridecanoic acid	214	C13H26O2	000638-53-9	58
5		Tetradecane	198	C14H30	000629-59-4	53

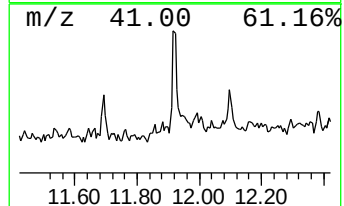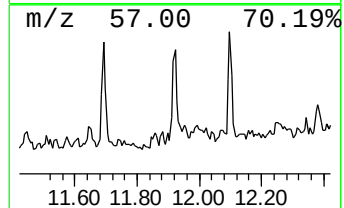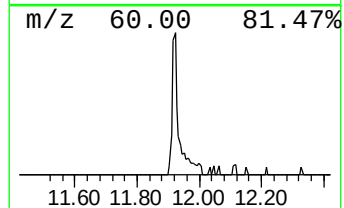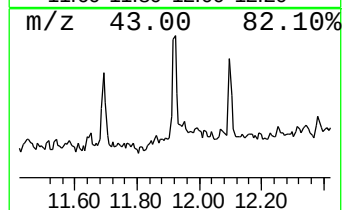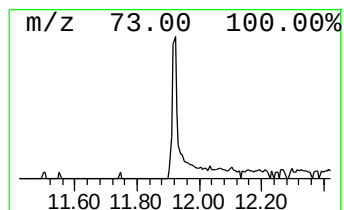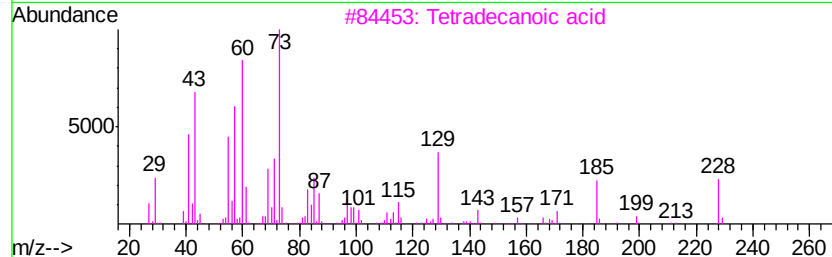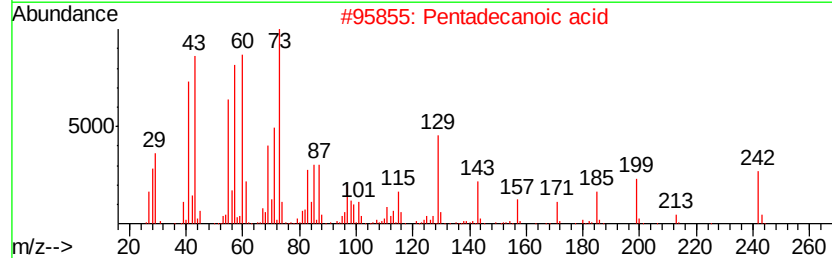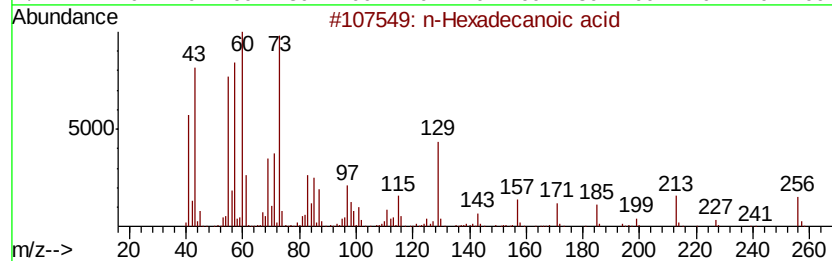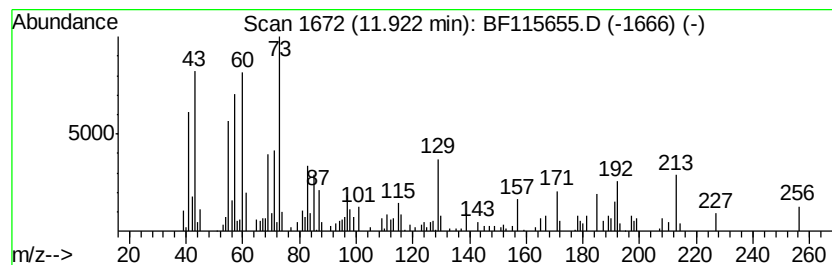

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Benzene, 1,1'-(1,3-butadiyn... Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.84	2.46 ng	143457	Chrysene-d12	14.03
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Pyrene	202 C16H10	000129-00-0	95
2	Fluoranthene	202 C16H10	000206-44-0	83
3	Benzene, 1,1'-(1,3-butadiyne-1,4...	202 C16H10	000886-66-8	53
4	Anthracene, 9-(2-nitroethenyl)-	249 C16H11N02	058349-77-2	38
5	l-Leucyl-l-leucine, N,N'-dimethy...	528 C29H56N2O6	1000328-59-7	28

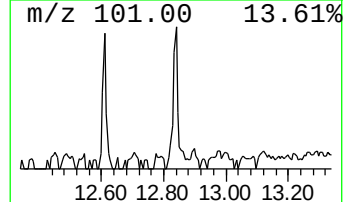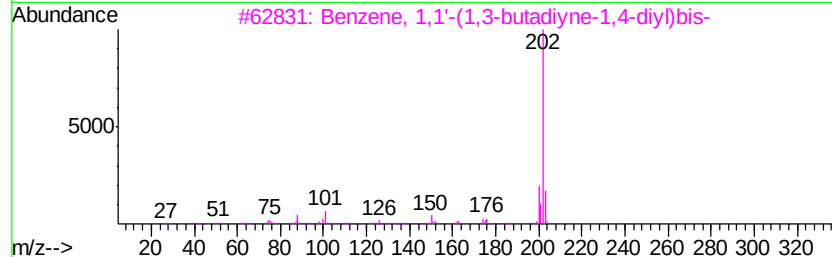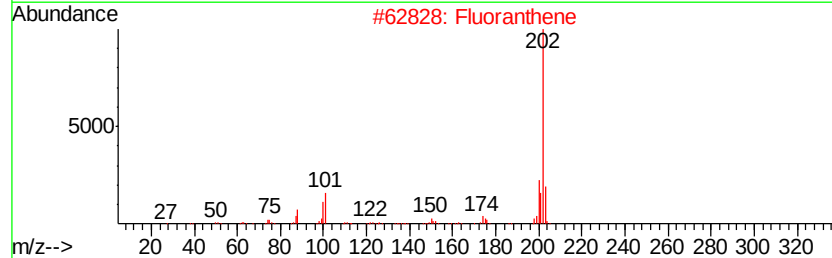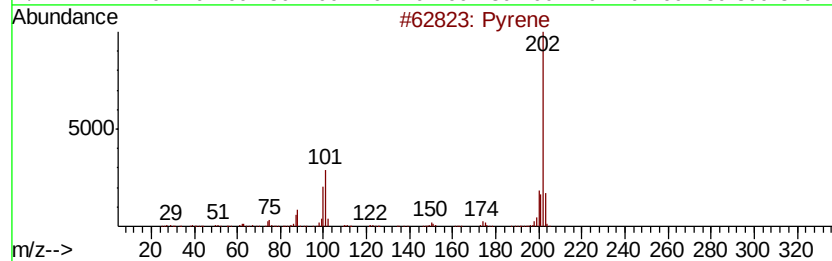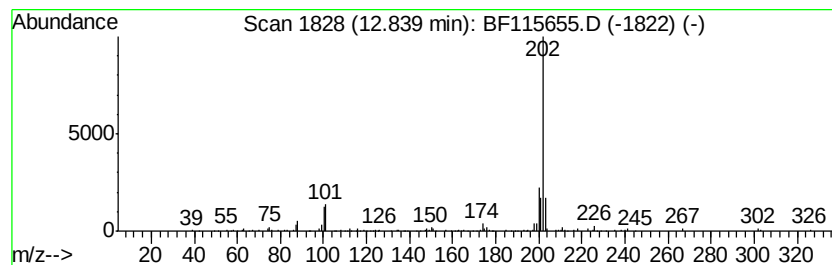

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 unknown13.56 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.56	3.28 ng	191510	Chrysene-d12	14.03

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopropanemethanol, .alpha.,2-...	182	C12H22O	121959-70-4	38
2		2-Cyclohexene-1-carboxaldehyde, ...	220	C15H24O	056772-07-7	30
3		E-11-Methyl-12-tetradecen-1-ol a...	268	C17H32O2	1000130-80-7	25
4		2-Acetoxy-1,1,10-trimethyl-6,9-e...	268	C15H24O4	108511-84-8	22
5		4-Methyl-Z-4-hexadecen-1-ol	254	C17H34O	1000130-89-0	22

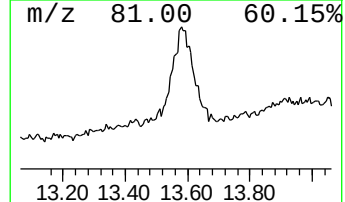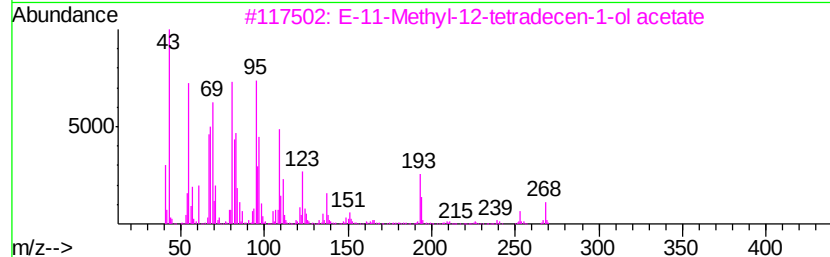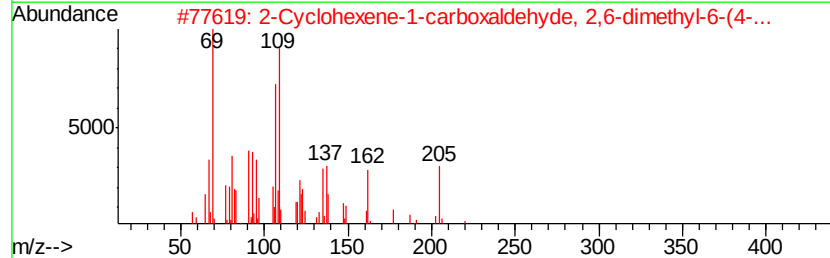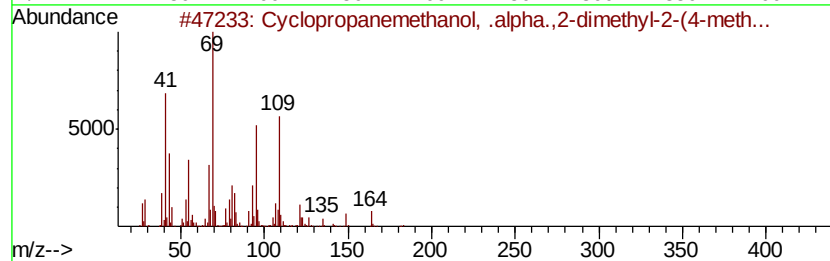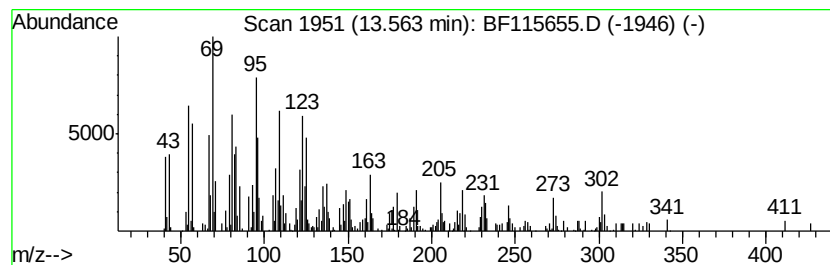

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071819\
Data File : BF115655.D
Acq On : 18 Jul 2019 18:45
Operator : HP/JU
Sample : K3615-05 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-071719-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.15	5.9	ng	280585	1	6.89	950793	20.0
unknown6.65	6.65	24.5	ng	1165790	1	6.89	950793	20.0
Tridecane	8.76	2.2	ng	163135	2	8.16	1455850	20.0
Nonadecane	9.32	2.5	ng	150510	3	9.92	1206740	20.0
n-Hexadecanoic acid	11.92	2.1	ng	117204	4	11.40	1136920	20.0
Benzene, 1,1'-(1,...	12.84	2.5	ng	143457	5	14.03	1167500	20.0
unknown13.56	13.56	3.3	ng	191510	5	14.03	1167500	20.0