


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071819\
 Data File : BF115640.D
 Acq On : 18 Jul 2019 8:02
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

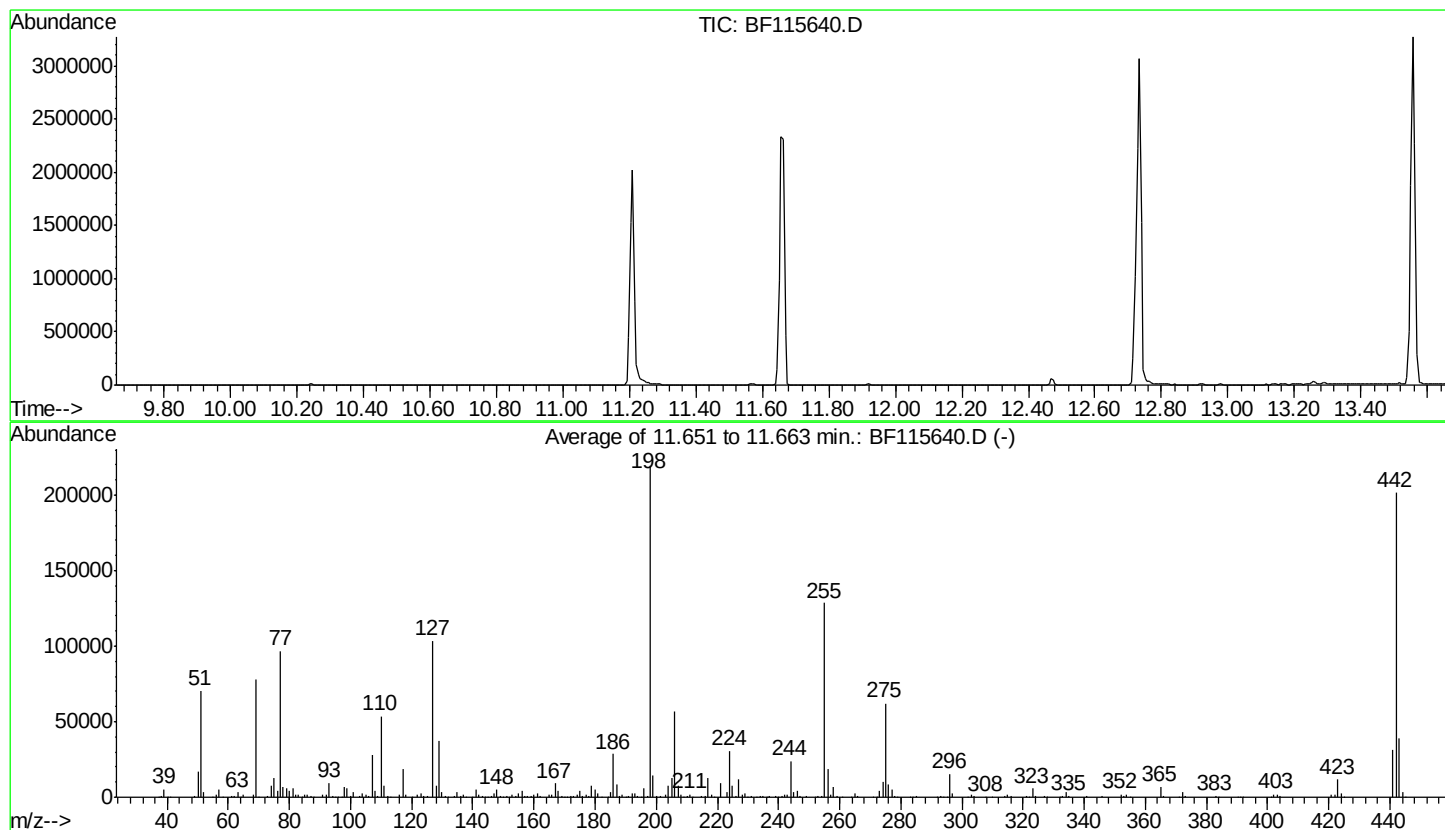

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	70536	PASS
68	69	0.00	2	1.8	1380	PASS
69	198	0.00	100	35.6	78245	PASS
70	69	0.00	2	0.4	301	PASS
127	198	10	80	47.3	103832	PASS
197	198	0.00	2	0.4	852	PASS
198	198	100	100	100.0	219536	PASS
199	198	5	9	6.7	14653	PASS
275	198	10	60	28.3	62048	PASS
365	198	1	100	3.2	7117	PASS
441	198	0.01	100	14.5	31765	PASS
442	198	50	100	91.7	201341	PASS
443	442	15	24	19.2	38604	PASS