


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF071819\  
 Data File : BF115656.D  
 Acq On : 18 Jul 2019 20:32  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF071219.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 12 14:03:52 2019

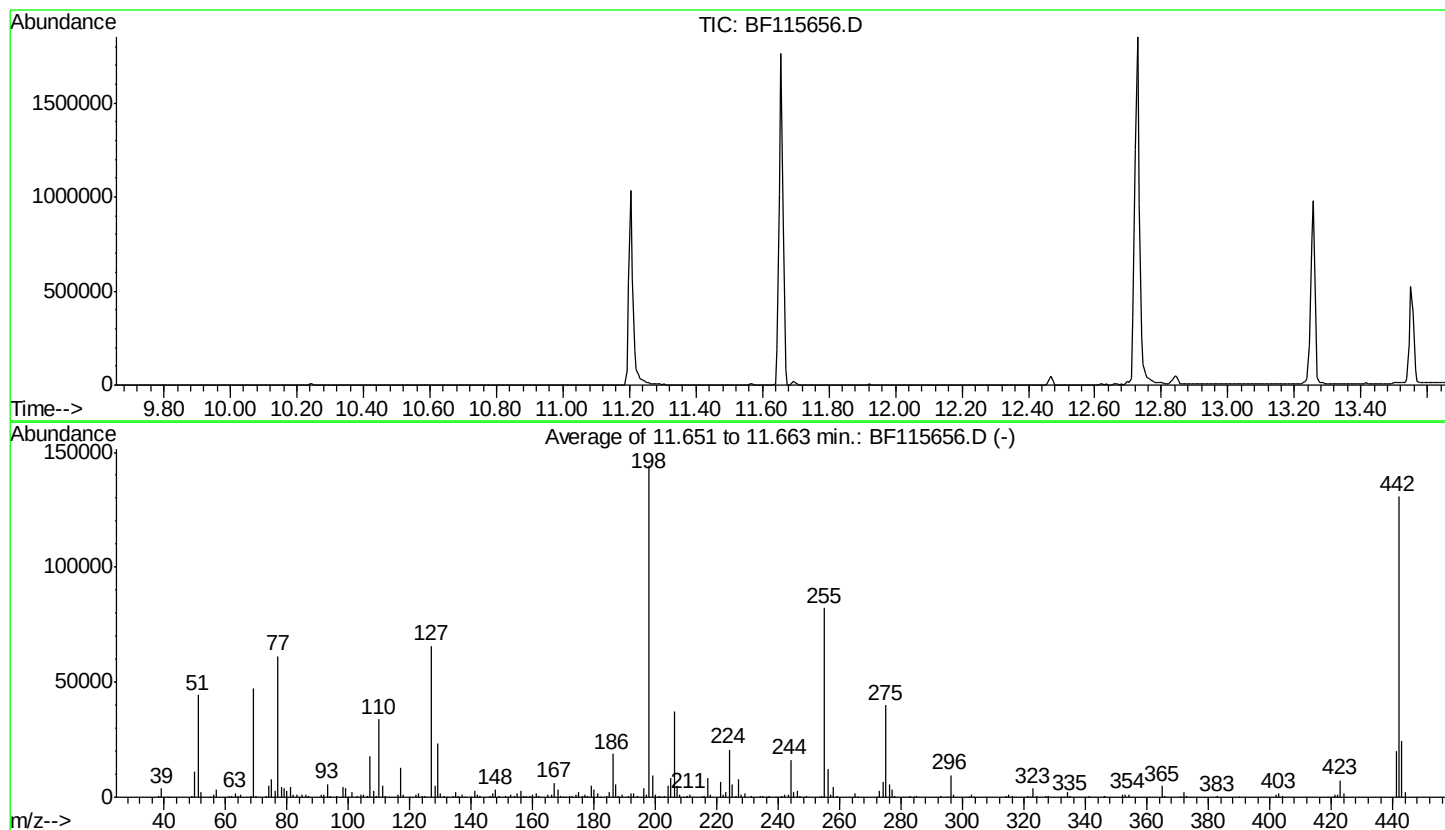

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 30.9      | 44517   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 786     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.0      | 47506   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 304     | PASS             |
| 127         | 198          | 10           | 80           | 45.6      | 65706   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 971     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 144168  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 9680    | PASS             |
| 275         | 198          | 10           | 60           | 27.6      | 39850   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 4982    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.0      | 20125   | PASS             |
| 442         | 198          | 50           | 100          | 90.5      | 130533  | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 24622   | PASS             |