
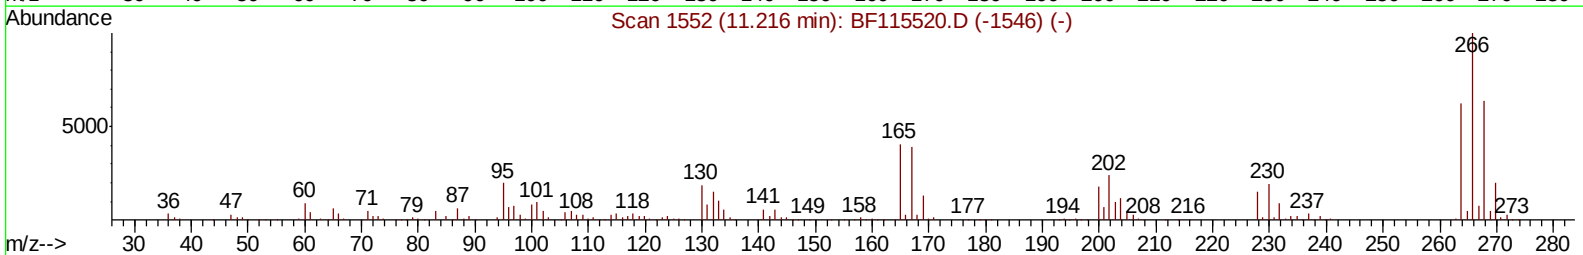
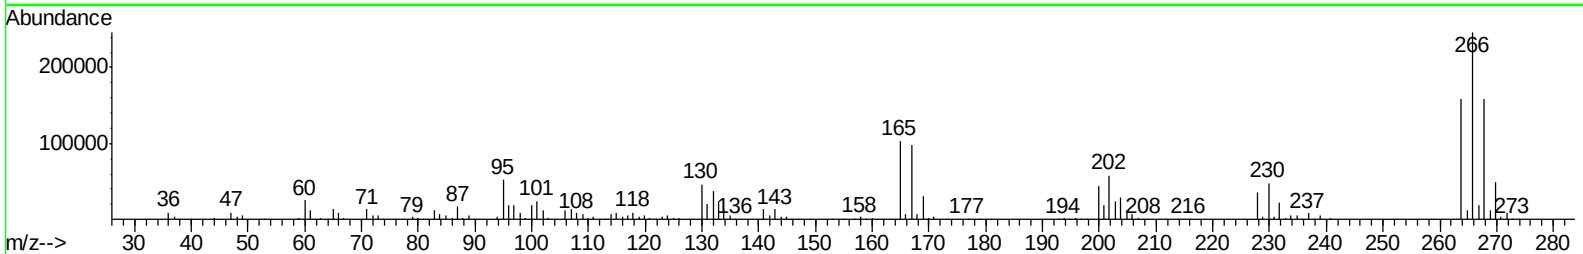


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072219\
Data File : BF115699.D
Acq On : 22 Jul 2019 9:39
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:09:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

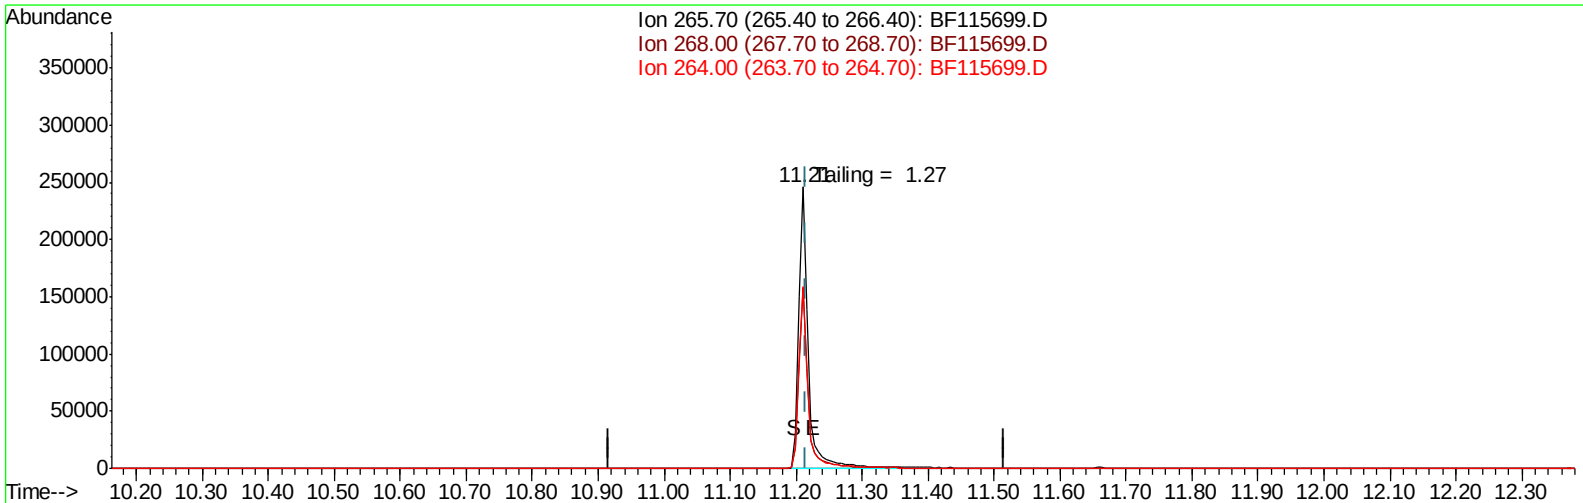

TIC: BF115699.D

(70) Pentachlorophenol (C)




11.210min (-0.006) 279554.63ng

response 249914

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.21
264.00	63.30	64.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072219\
Data File : BF115699.D
Acq On : 22 Jul 2019 9:39
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:09:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

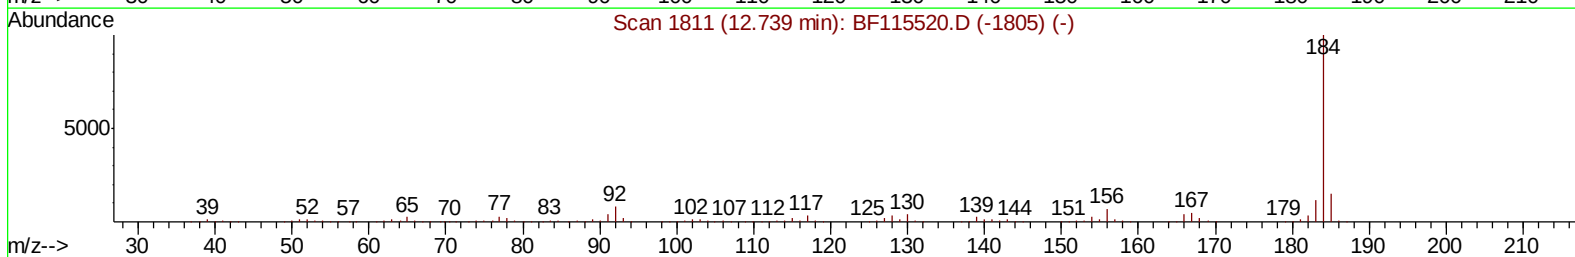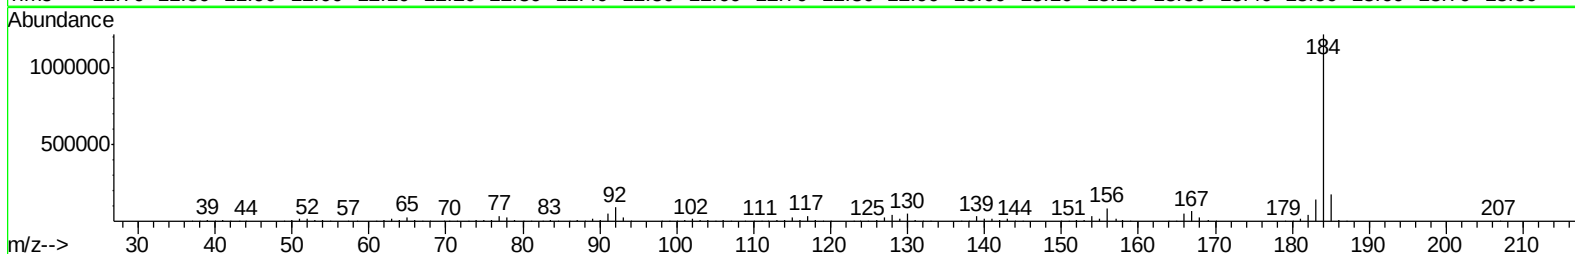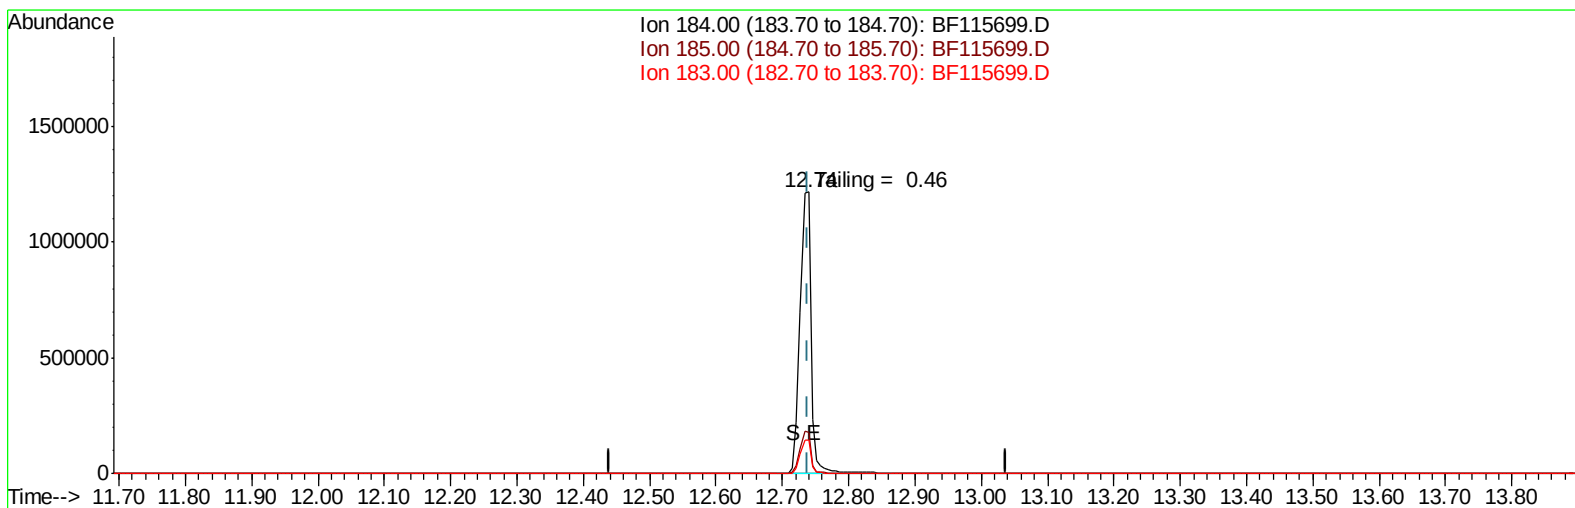

TIC: BF115699.D

(77) Benzidine

12.739min (-0.000) 0.00ng

response 1350493

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.59
183.00	11.60	11.94
0.00	0.00	0.00