

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072219\
 Data File : BF115707.D
 Acq On : 22 Jul 2019 14:13
 Operator : HP/JU
 Sample : PB121584BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121584BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.251	15	28	35	rVB	88617	132921	2.09%	0.286%
2	5.510	577	582	586	rBV	3980635	4611493	72.55%	9.915%
3	6.516	746	753	755	rBV	3973396	4806085	75.62%	10.334%
4	6.651	771	776	779	rBV	4595029	4945850	77.81%	10.634%
5	6.875	811	814	818	rBV	1200681	1097967	17.27%	2.361%
6	7.039	837	842	845	rBV	3918768	3990592	62.79%	8.580%
7	7.439	904	910	913	rBV	2938101	3243505	51.03%	6.974%
8	8.157	1027	1032	1048	rBV	1350025	1403107	22.08%	3.017%
9	9.239	1209	1216	1219	rBV	5574065	5943511	93.51%	12.779%
10	9.916	1325	1331	1343	rBV	1878502	1695314	26.67%	3.645%
11	10.704	1460	1465	1493	rBV	3386763	3828748	60.24%	8.232%
12	11.398	1579	1583	1591	rBV	1769306	1712440	26.94%	3.682%
13	12.992	1848	1854	1857	rBV	5746100	6355909	100.00%	13.666%
14	13.892	1992	2007	2016	rBV2	33575	123958	1.95%	0.267%
15	14.039	2028	2032	2043	rBV	1436495	1374098	21.62%	2.954%
16	15.515	2277	2283	2298	rBV	798104	1155457	18.18%	2.484%
17	16.780	2490	2498	2510	rVB7	22942	87801	1.38%	0.189%


Sum of corrected areas: 46508756

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072219\
Data File : BF115707.D
Acq On : 22 Jul 2019 14:13
Operator : HP/JU
Sample : PB121584BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121584BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

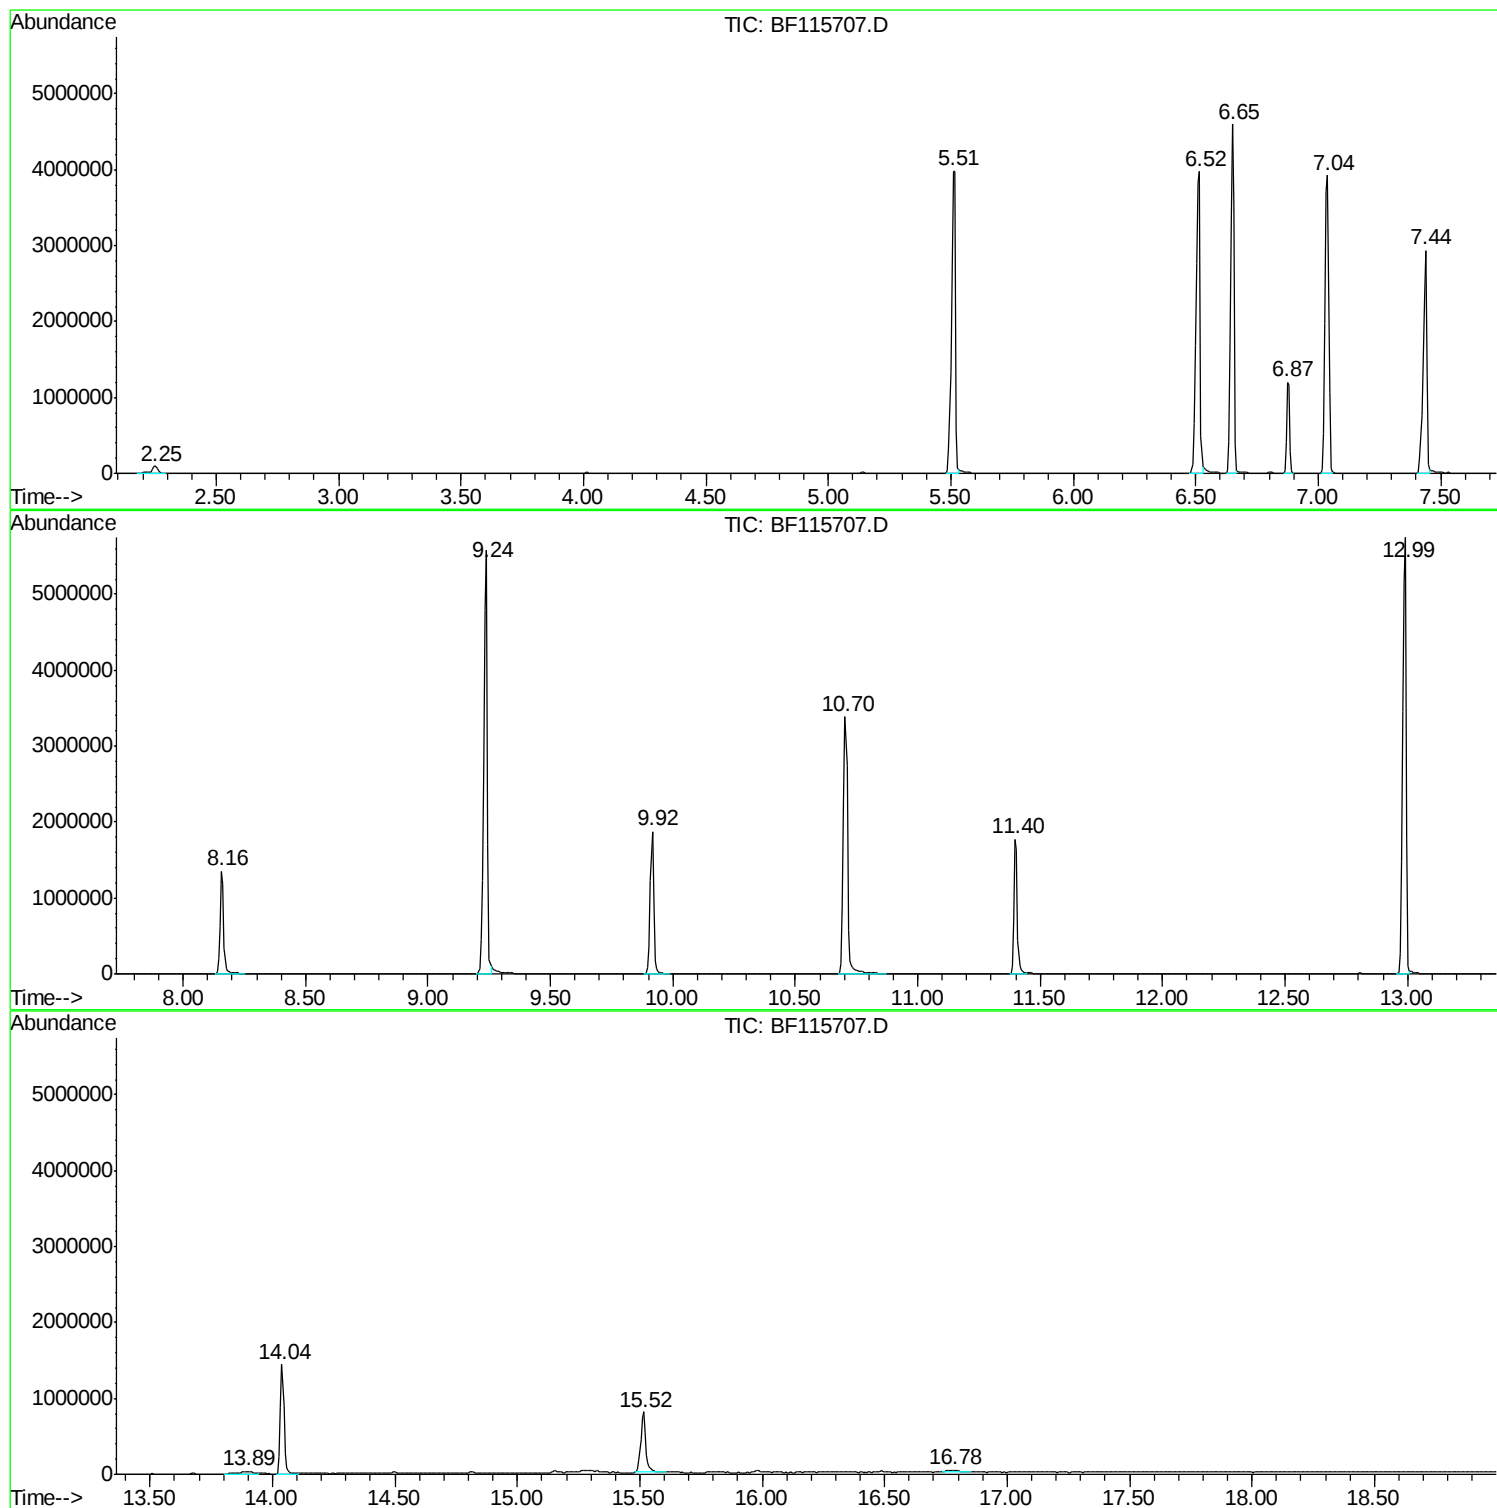

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072219\
Data File : BF115707.D
Acq On : 22 Jul 2019 14:13
Operator : HP/JU
Sample : PB121584BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121584BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.25	2.42 ng	132921	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	56
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

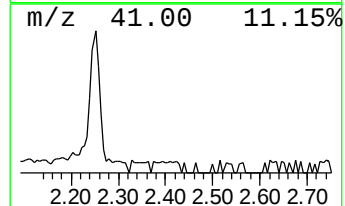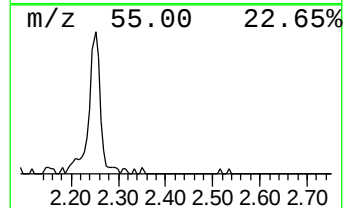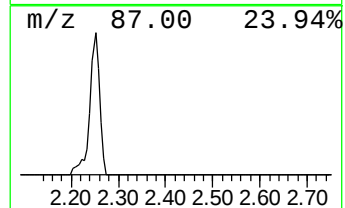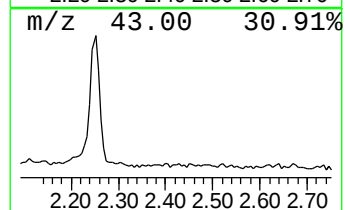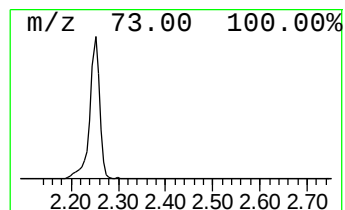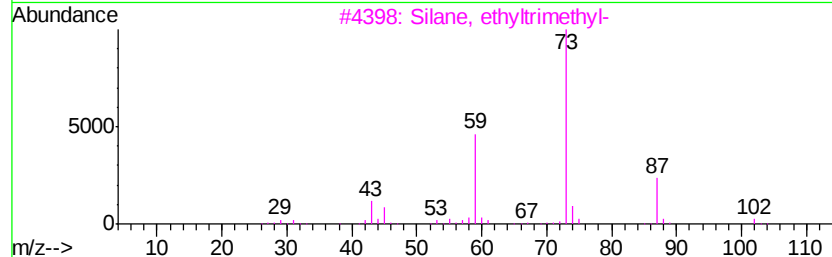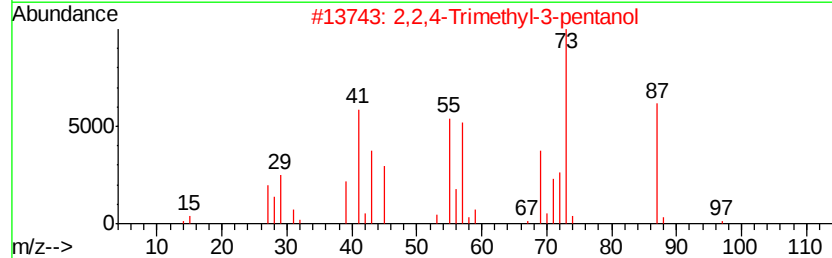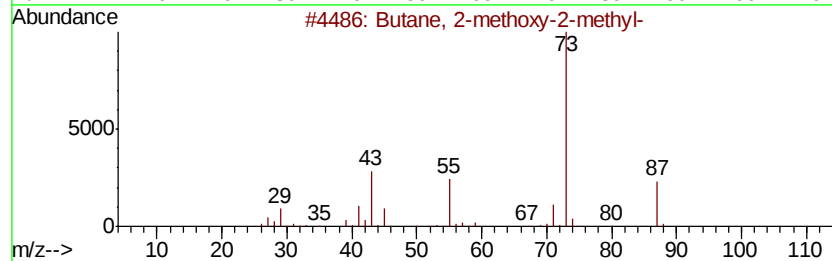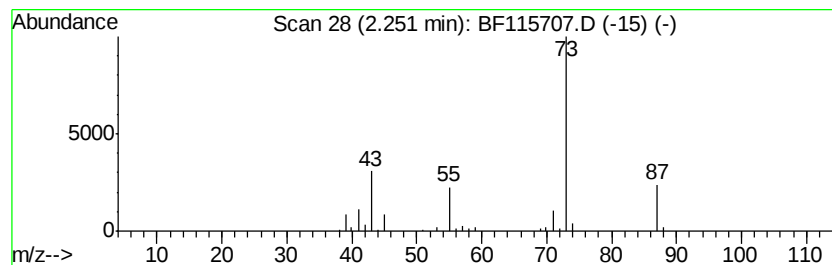

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072219\
Data File : BF115707.D
Acq On : 22 Jul 2019 14:13
Operator : HP/JU
Sample : PB121584BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121584BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	90.09 ng	4945850	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Xenon	132	Xe	007440-63-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

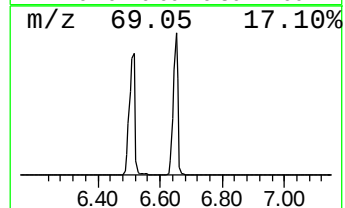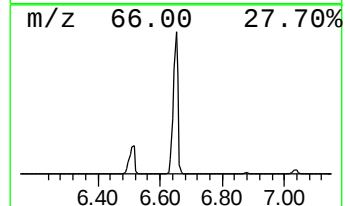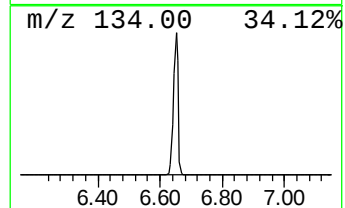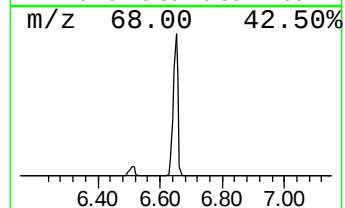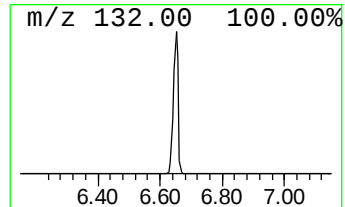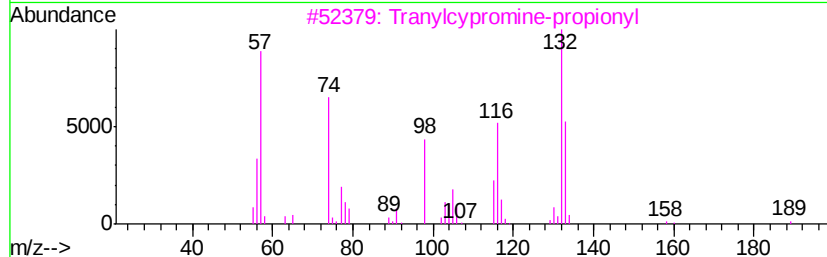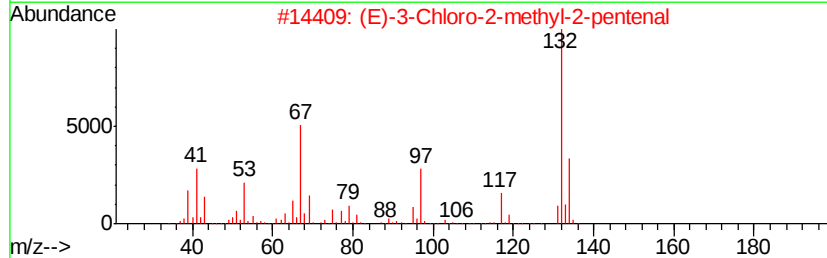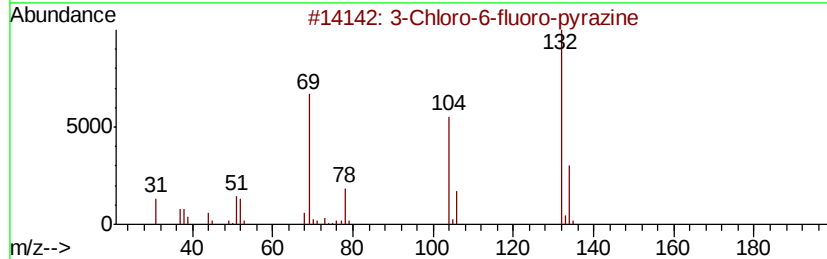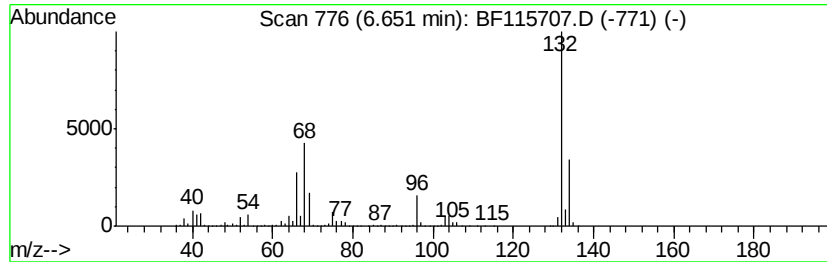

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072219\
Data File : BF115707.D
Acq On : 22 Jul 2019 14:13
Operator : HP/JU
Sample : PB121584BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121584BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.25	2.4	ng	132921	1	6.88	1097970	20.0
unknown6.65	6.65	90.1	ng	4945850	1	6.88	1097970	20.0