


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF072219\  
 Data File : BF115699.D  
 Acq On : 22 Jul 2019 9:39  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF071219.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 12 14:03:52 2019

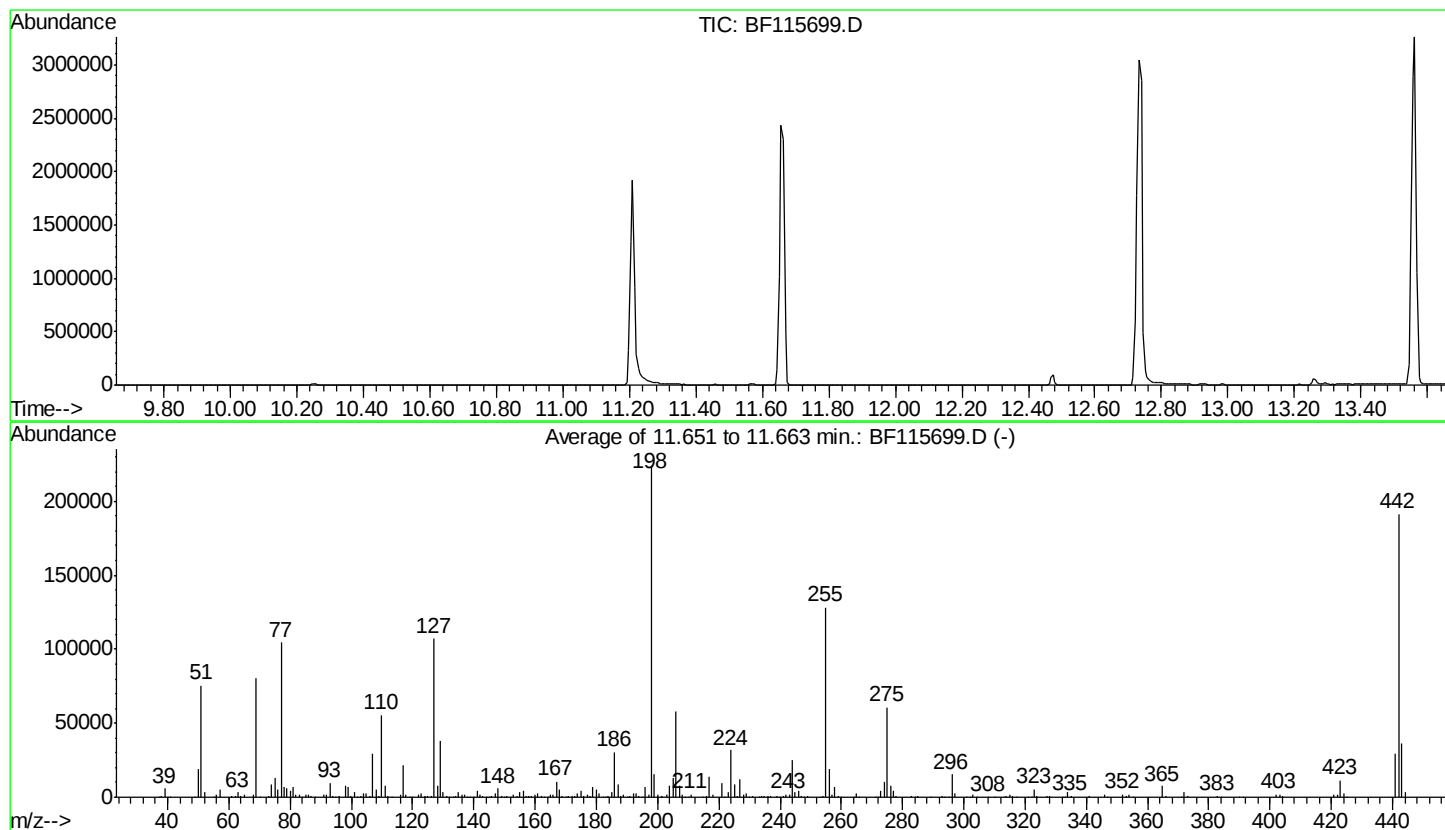

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.7      | 75554   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 1335    | PASS             |
| 69          | 198          | 0.00         | 100          | 35.9      | 80354   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 451     | PASS             |
| 127         | 198          | 10           | 80           | 47.8      | 107080  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 1395    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 224013  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 15265   | PASS             |
| 275         | 198          | 10           | 60           | 27.0      | 60562   | PASS             |
| 365         | 198          | 1            | 100          | 3.3       | 7451    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.2      | 29539   | PASS             |
| 442         | 198          | 50           | 100          | 85.4      | 191322  | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 36762   | PASS             |