
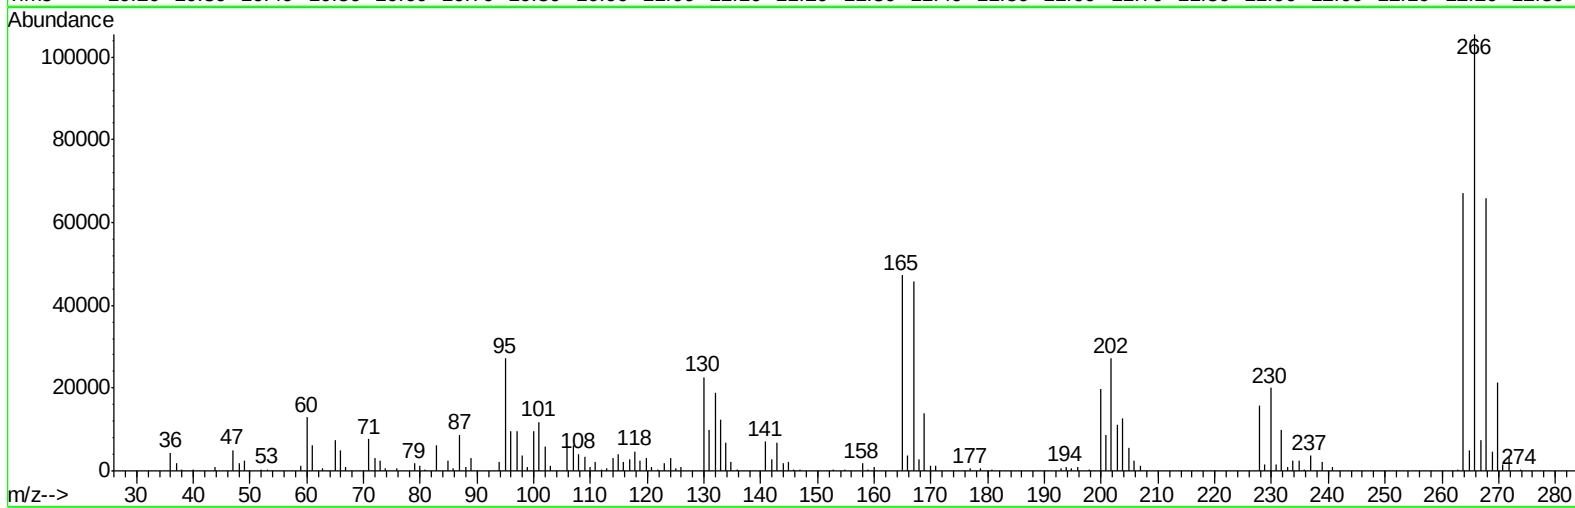


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072319\
Data File : BF115718.D
Acq On : 23 Jul 2019 14:06
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 08:44:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

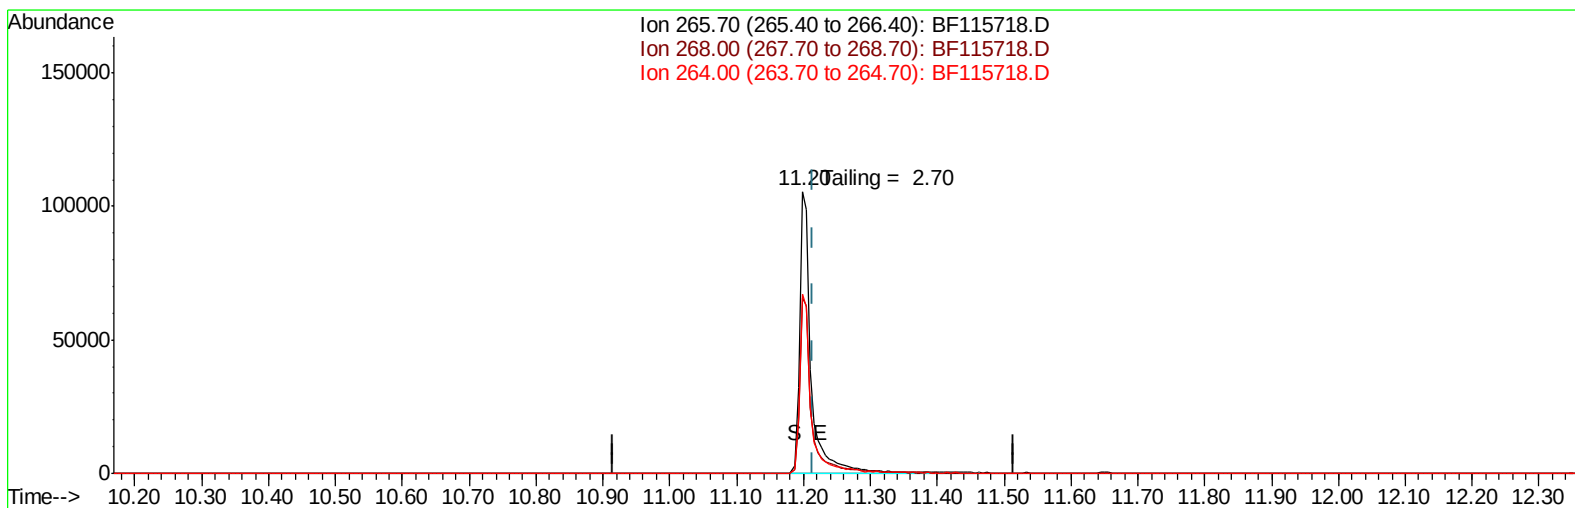

TIC: BF115718.D

(70) Pentachlorophenol (C)



11.198min (-0.018) 25384.74ng

response 128460

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.39
264.00	63.30	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072319\
Data File : BF115718.D
Acq On : 23 Jul 2019 14:06
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 08:44:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

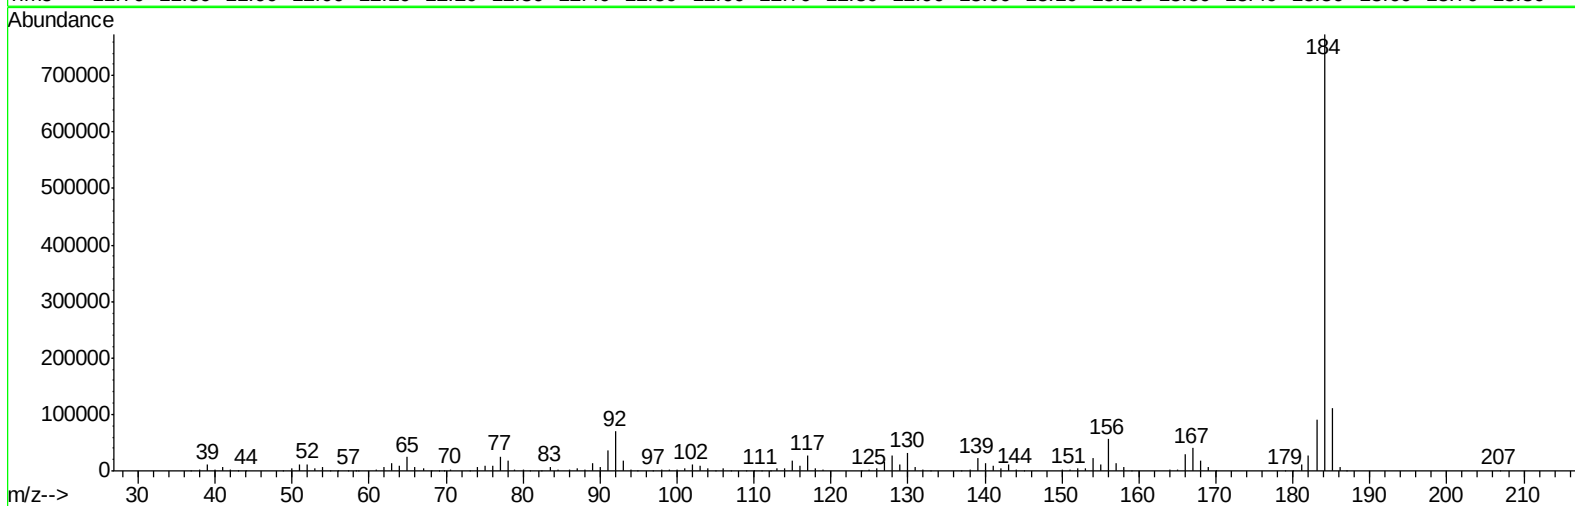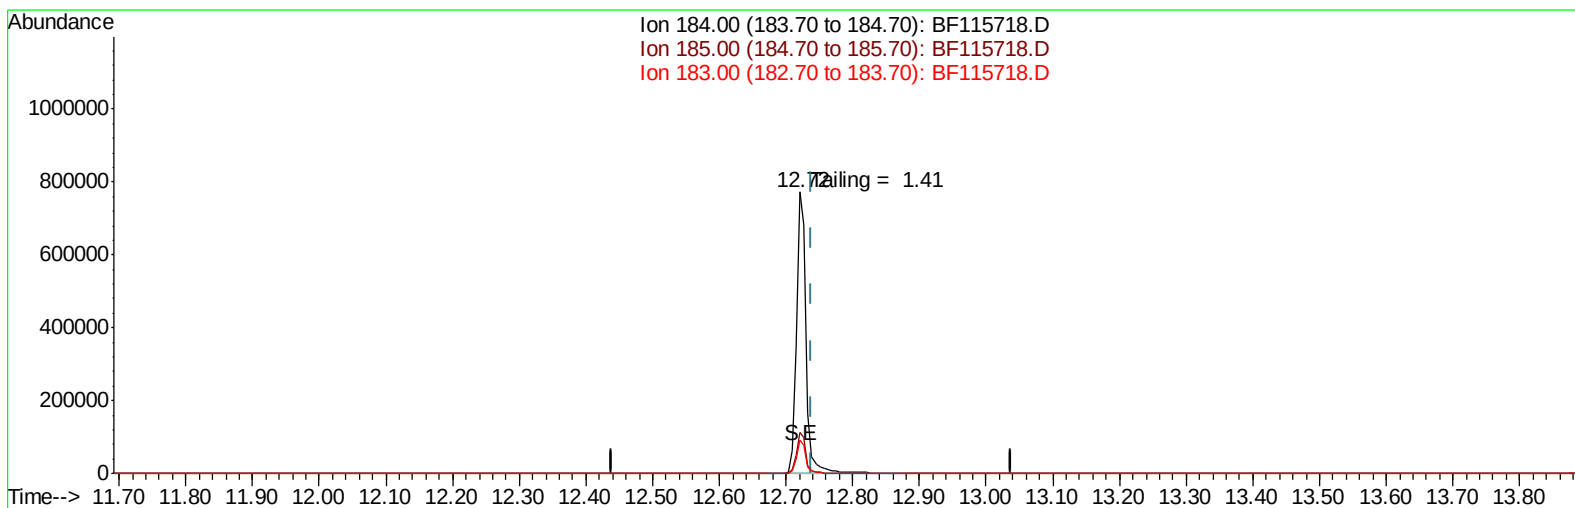

TIC: BF115718.D

(77) Benzidine

12.721min (-0.018) 0.00ng

response 773978

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.45
183.00	11.60	11.67
0.00	0.00	0.00