


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072319\
 Data File : BF115718.D
 Acq On : 23 Jul 2019 14:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 14:03:52 2019

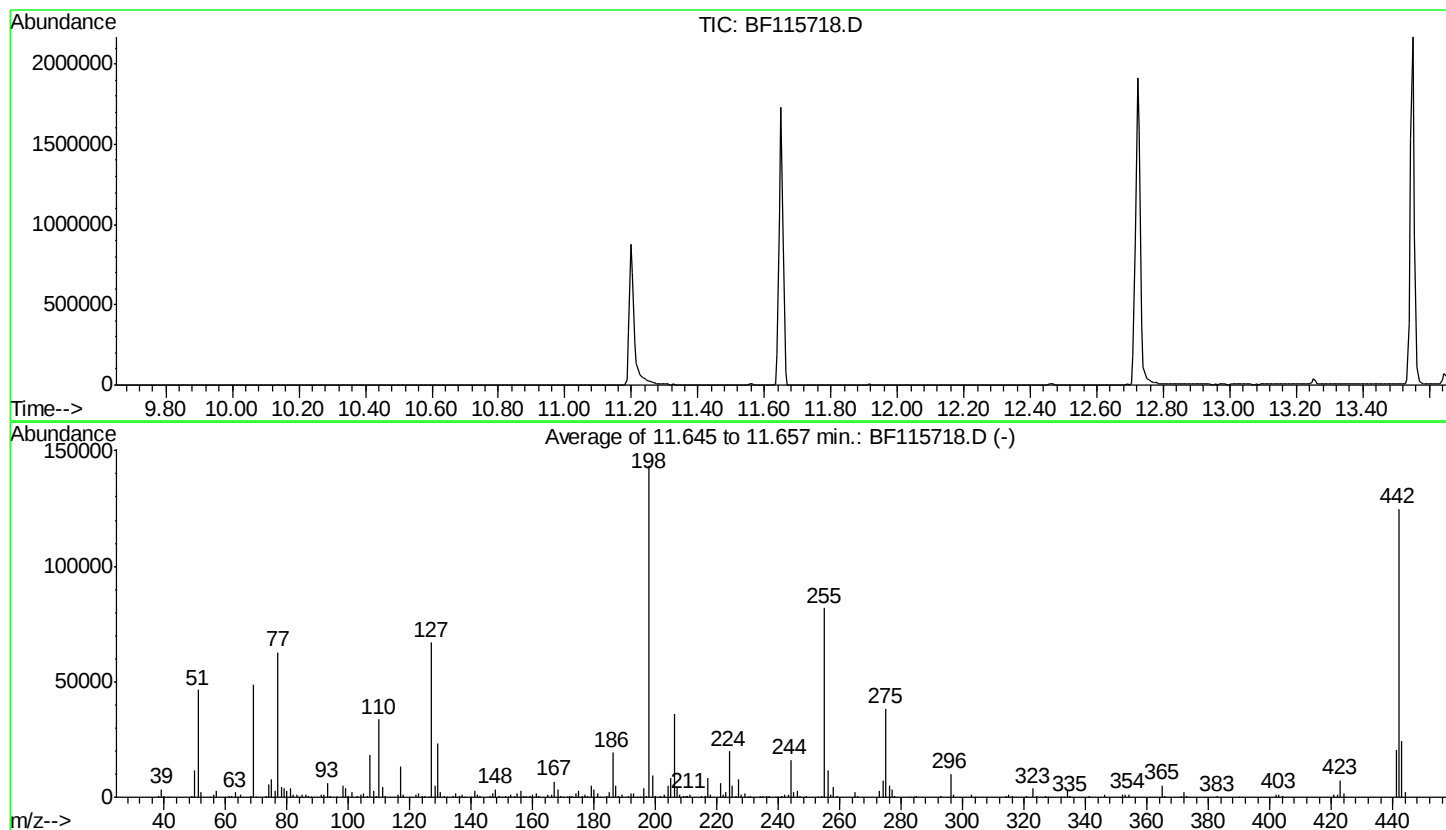

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	46312	PASS
68	69	0.00	2	1.7	829	PASS
69	198	0.00	100	34.0	48861	PASS
70	69	0.00	2	0.3	160	PASS
127	198	10	80	46.6	66906	PASS
197	198	0.00	2	0.5	756	PASS
198	198	100	100	100.0	143573	PASS
199	198	5	9	6.6	9531	PASS
275	198	10	60	26.8	38426	PASS
365	198	1	100	3.6	5141	PASS
441	198	0.01	100	14.3	20510	PASS
442	198	50	100	86.9	124813	PASS
443	442	15	24	19.6	24460	PASS