
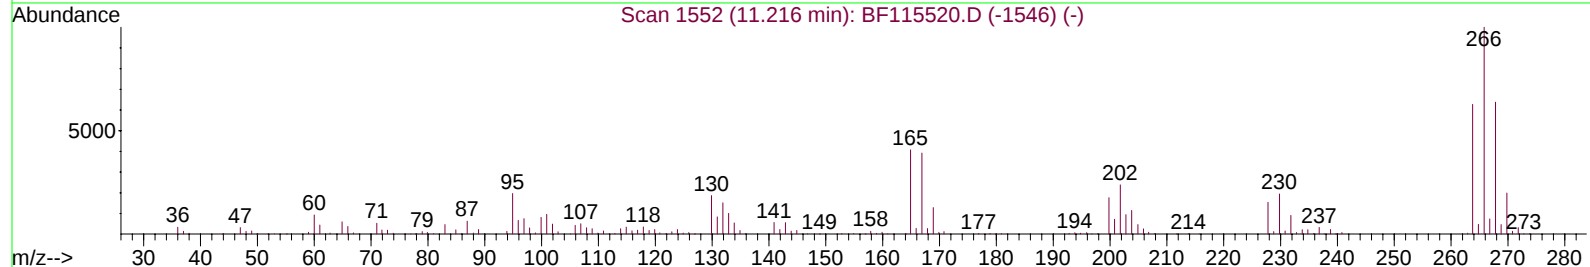
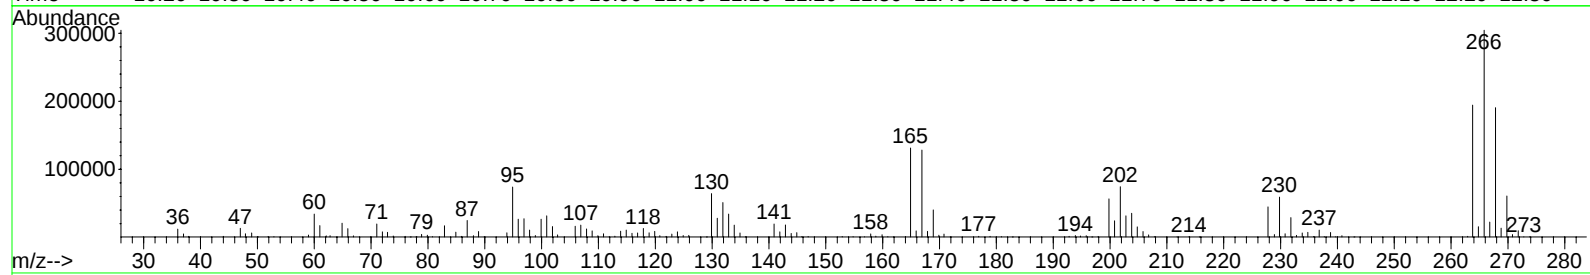


```

Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072919\
Data File   : BF115831.D
Acq On      : 29 Jul 2019   10:12
Operator    : HP/JU
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Jul 29 19:13:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 29 17:30:39 2019
Response via : Initial Calibration

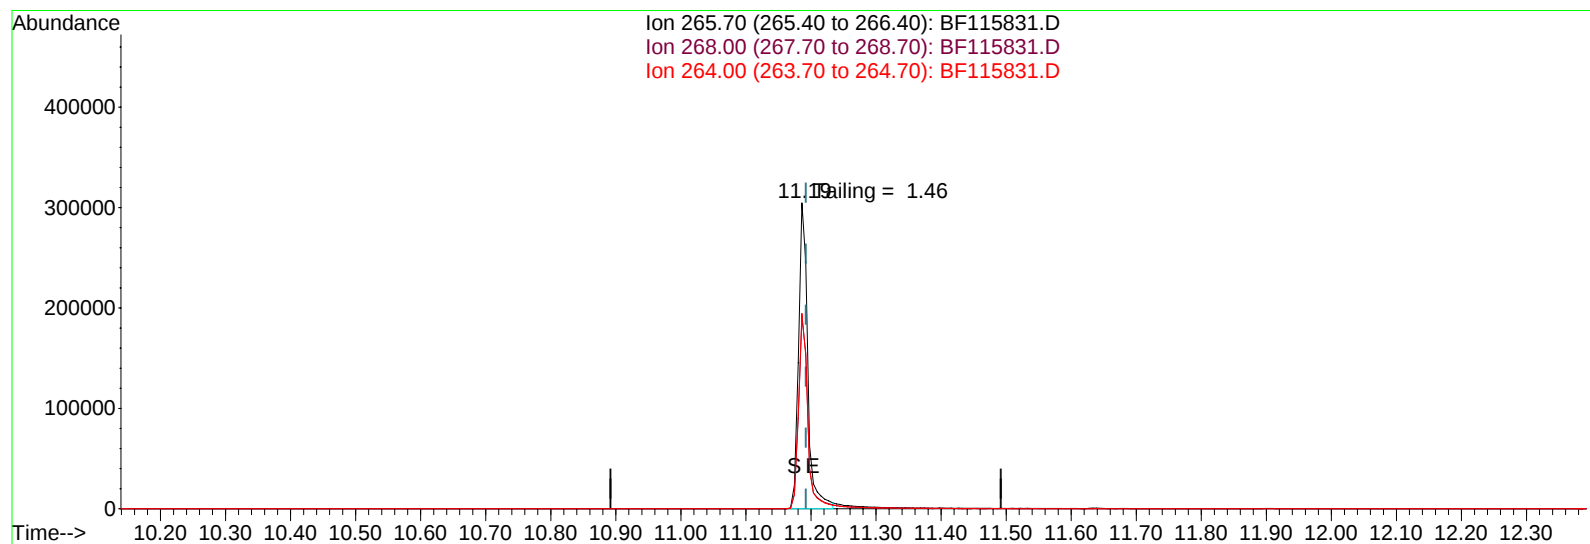

TIC: BF115831.D

(70) Pentachlorophenol (C)




11.186min (-0.006) 84390.12ng

response 319283

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	62.62
264.00	61.70	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072919\
Data File : BF115831.D
Acq On : 29 Jul 2019 10:12
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 19:13:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 29 17:30:39 2019
Response via : Initial Calibration

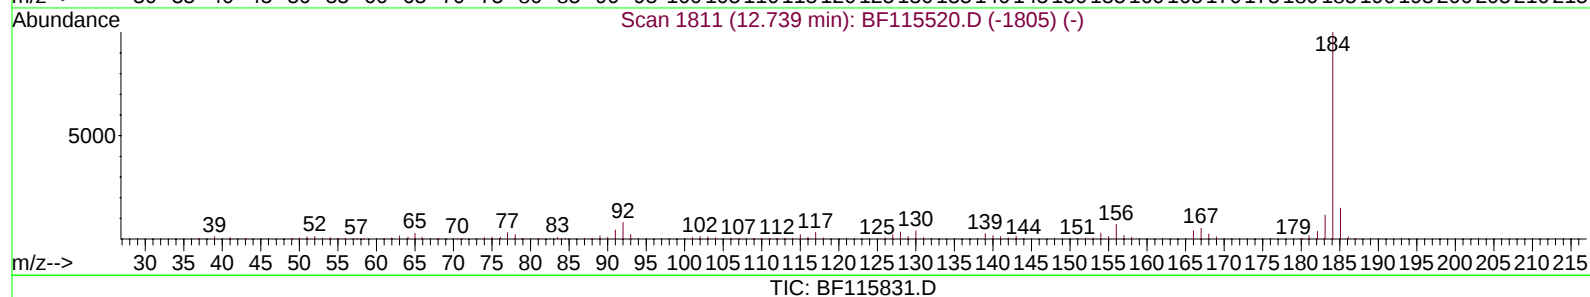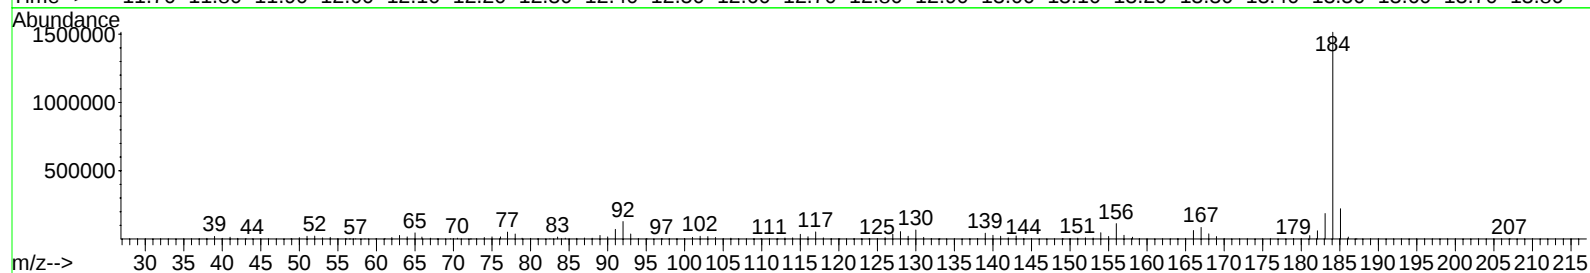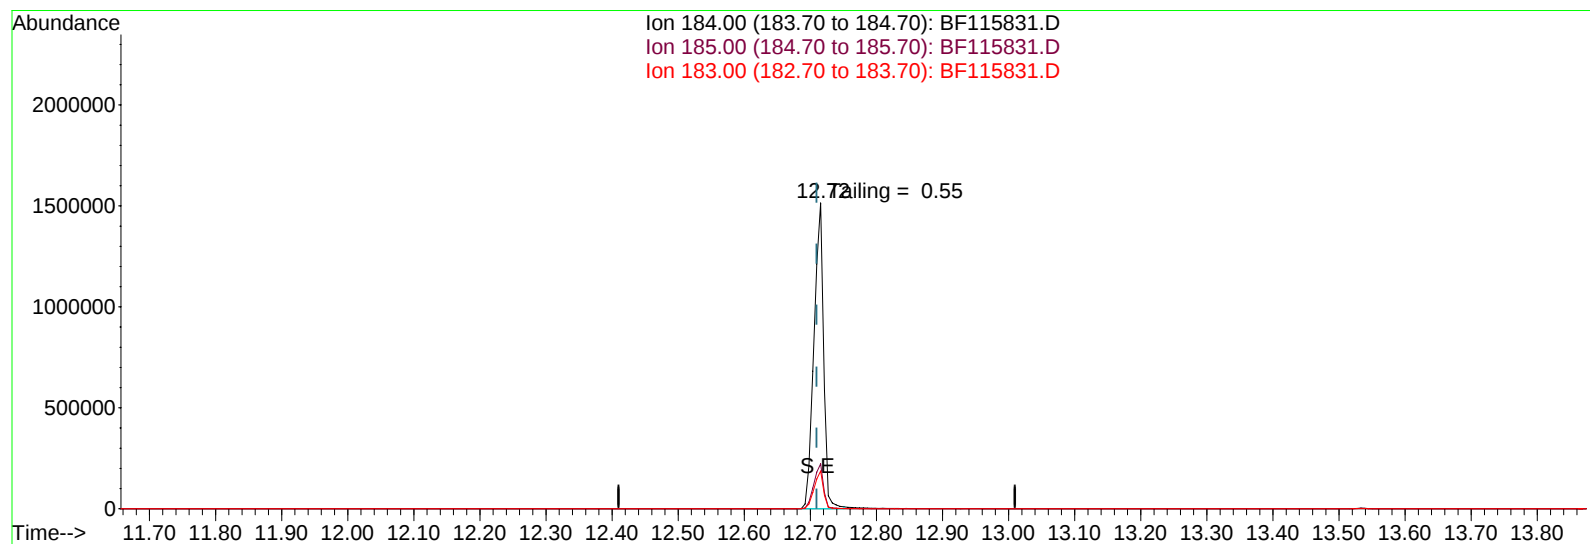

(77) Benzidine

12.715min (+0.006) 28972.72ng

response 1559049

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	11.40	12.34
0.00	0.00	0.00