


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072919\
 Data File : BF115831.D
 Acq On : 29 Jul 2019 10:12
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 29 17:30:39 2019

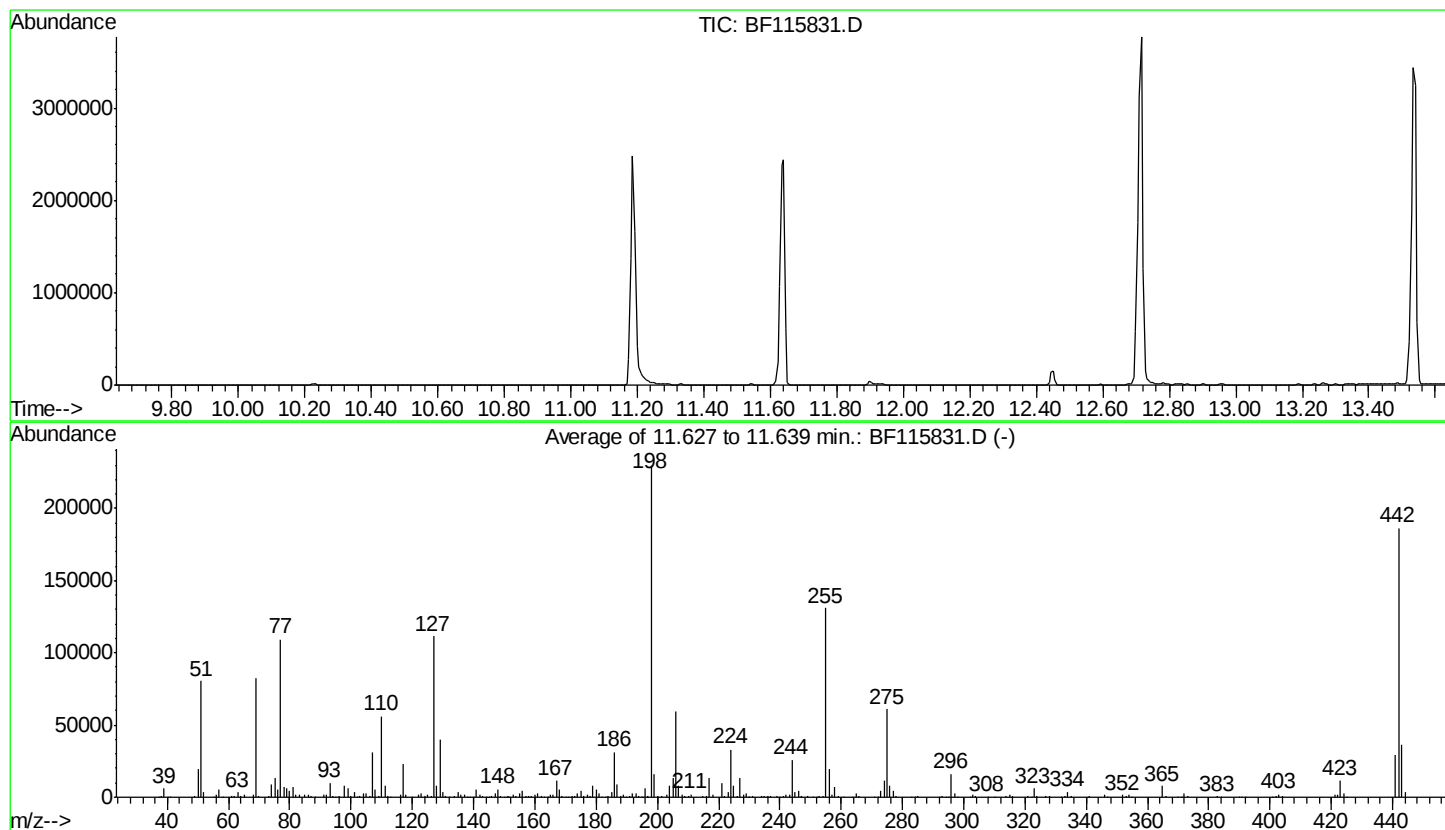

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	80602	PASS
68	69	0.00	2	1.8	1493	PASS
69	198	0.00	100	36.0	82752	PASS
70	69	0.00	2	0.6	472	PASS
127	198	10	80	48.6	111632	PASS
197	198	0.00	2	0.5	1145	PASS
198	198	100	100	100.0	229624	PASS
199	198	5	9	6.8	15567	PASS
275	198	10	60	26.6	61098	PASS
365	198	1	100	3.4	7856	PASS
441	198	0.01	100	12.7	29181	PASS
442	198	50	100	81.3	186610	PASS
443	442	15	24	19.6	36543	PASS