

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073119\
 Data File : BF115884.D
 Acq On : 31 Jul 2019 23:26
 Operator : HP/JU
 Sample : K4066-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-11

Quant Time: Aug 01 08:01:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:31:51 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	140344	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	517234	20.00	ng	0.00
39) Acenaphthene-d10	9.89	164	243146	20.00	ng	0.00
64) Phenanthrene-d10	11.38	188	367354	20.00	ng	0.00
76) Chrysene-d12	14.02	240	332303	20.00	ng	0.00
87) Perylene-d12	15.49	264	325765	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	734769	87.65	ng	0.00
7) Phenol-d6	6.49	99	953083	90.11	ng	0.00
23) Nitrobenzene-d5	7.41	82	573091	63.96	ng	0.00
42) 2,4,6-Tribromophenol	10.68	330	185290	78.60	ng	0.00
45) 2-Fluorobiphenyl	9.21	172	972955	74.95	ng	0.00
79) Terphenyl-d14	12.96	244	857849	54.40	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.60	163	156644	9.462	ng	99
75) Fluoranthene	12.59	202	40746	2.072	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073119\
Data File : BF115884.D
Acq On : 31 Jul 2019 23:26
Operator : HP/JU
Sample : K4066-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-11

Quant Time: Aug 01 08:01:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

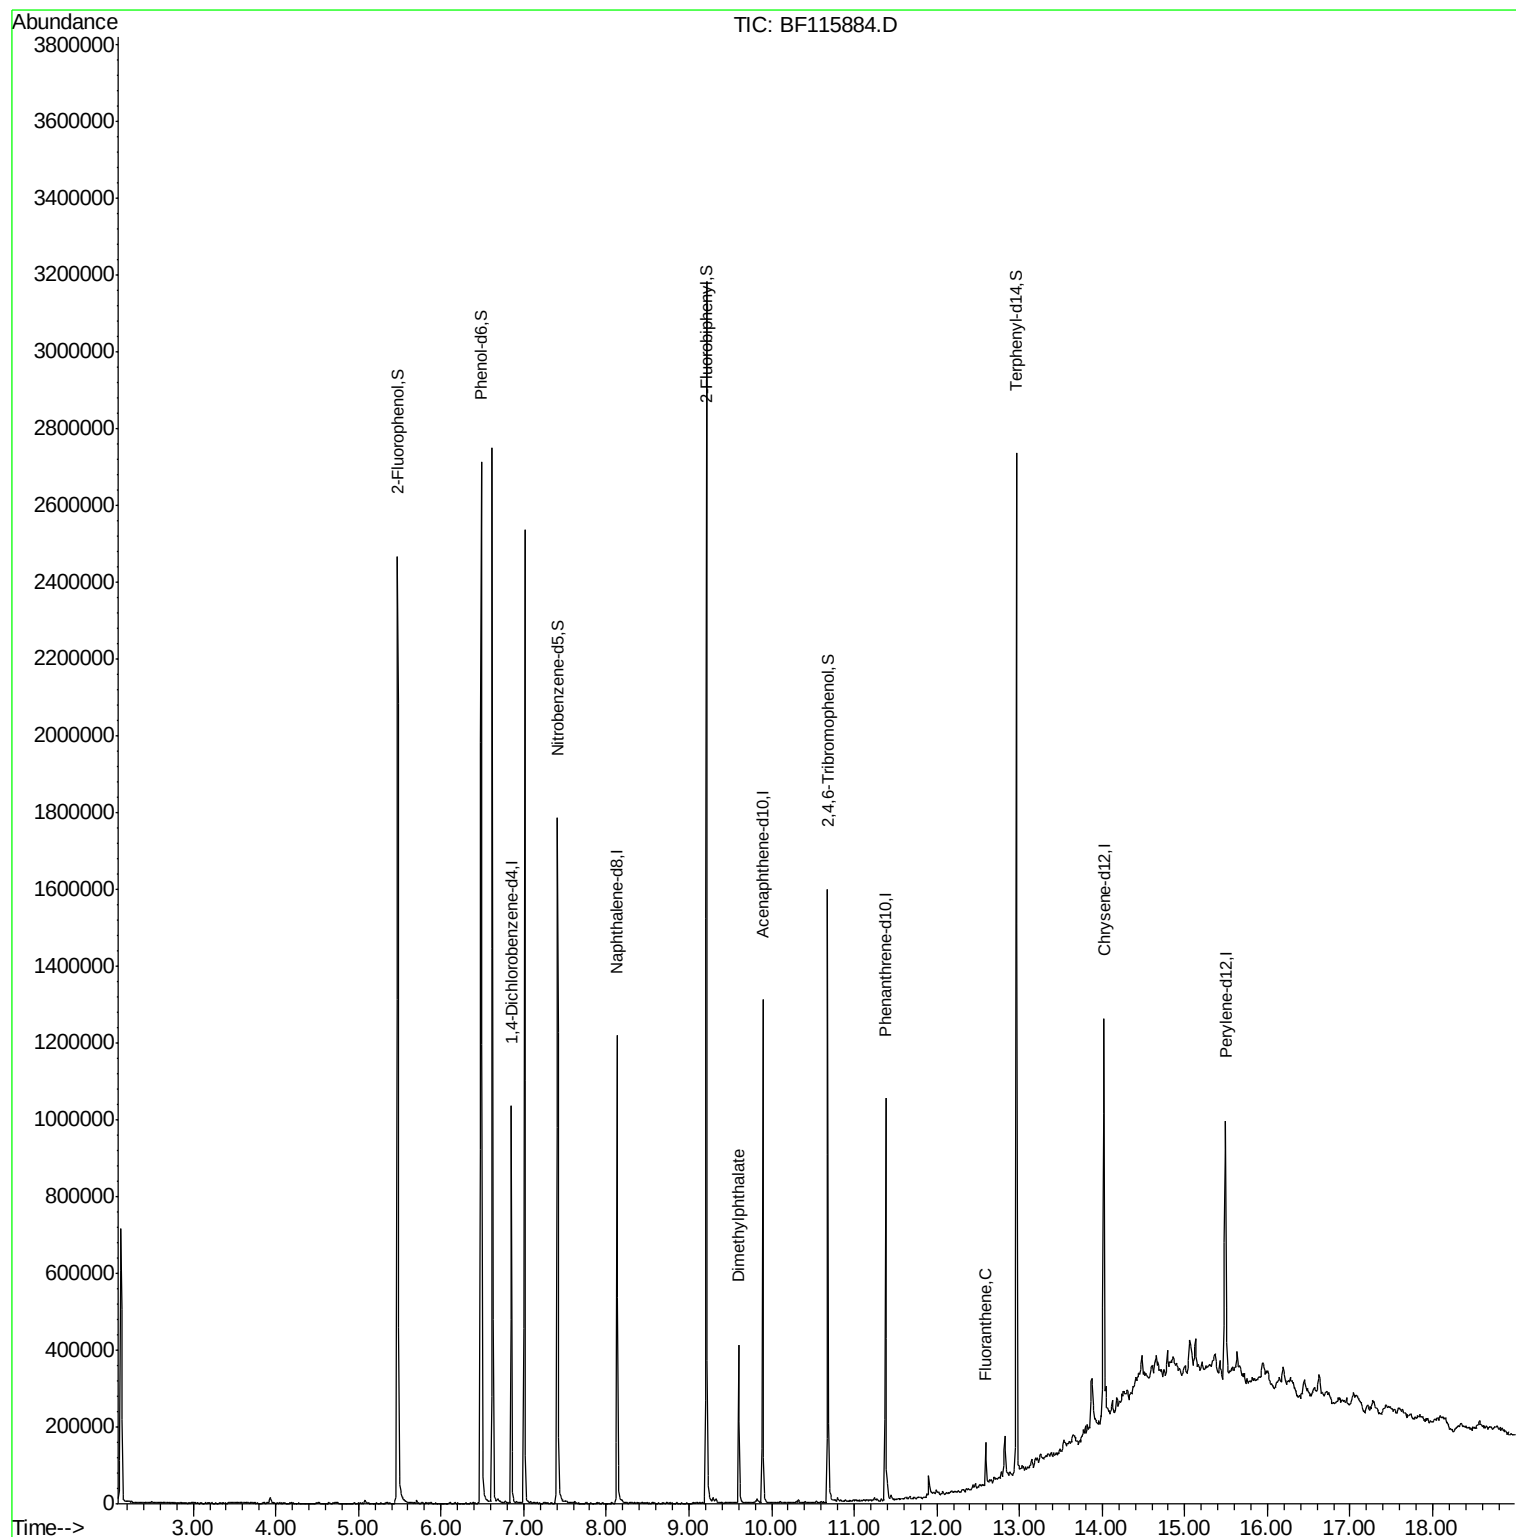

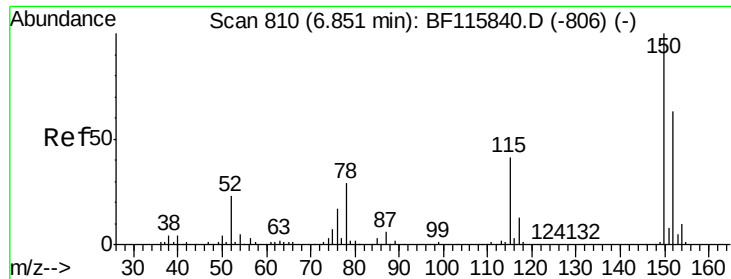


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 810
Delta R.T. 0.00 min
Lab File: BF115884.D
Acq: 31 Jul 2019 23:26

Instrument :
BNA_F
ClientSampleId :
TP-11

Tot Ion:152 Resp: 140344
Ion Ratio Lower Upper
152 100
150 155.1 127.4 191.0
115 62.4 51.8 77.8

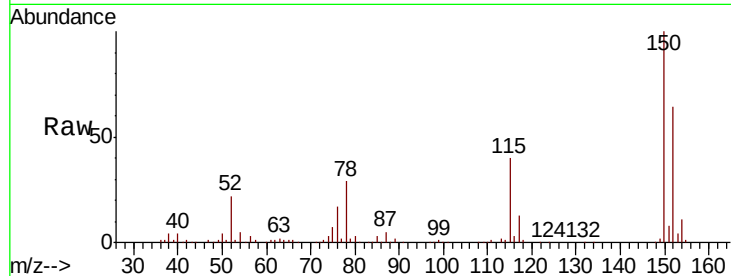


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

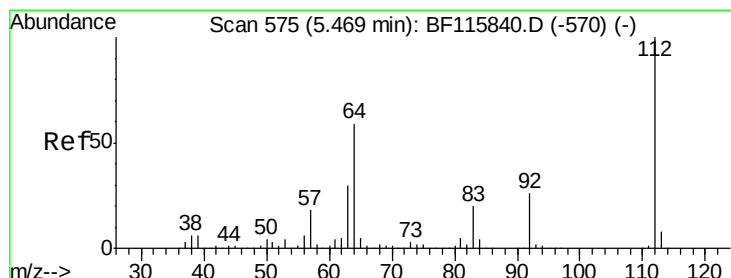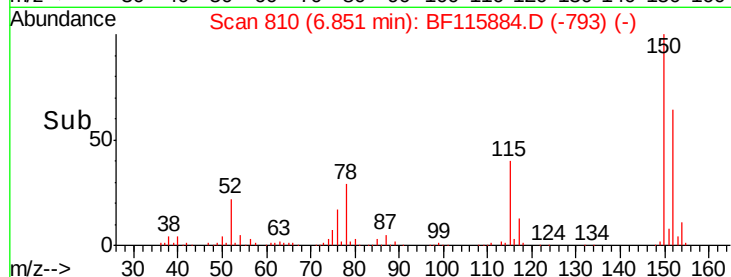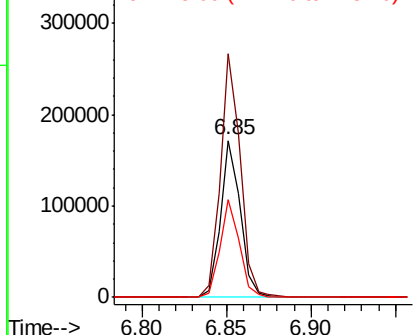



#5


2-Fluorophenol
Concen: 87.645 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.01 min
Lab File: BF115884.D
Acq: 31 Jul 2019 23:26

Tgt Ion:112 Resp: 734769
Ion Ratio Lower Upper
112 100
64 58.8 46.8 70.2
63 30.5 24.2 36.2

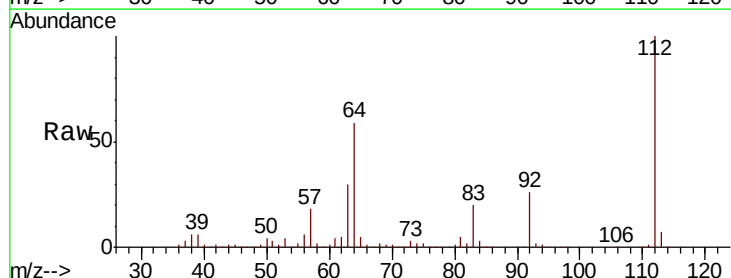

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

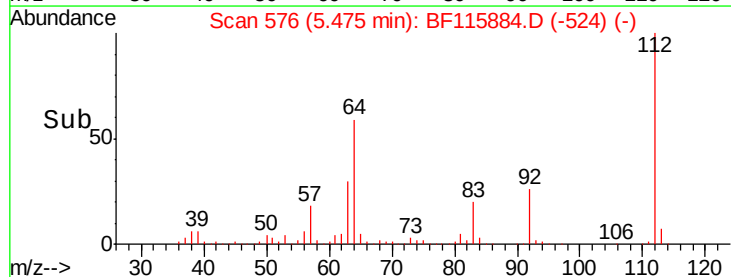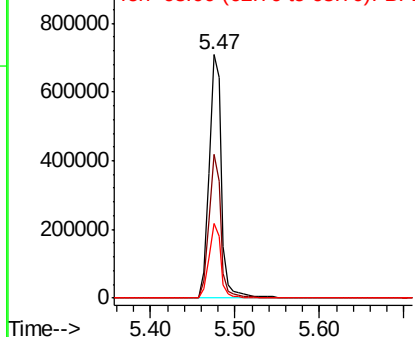

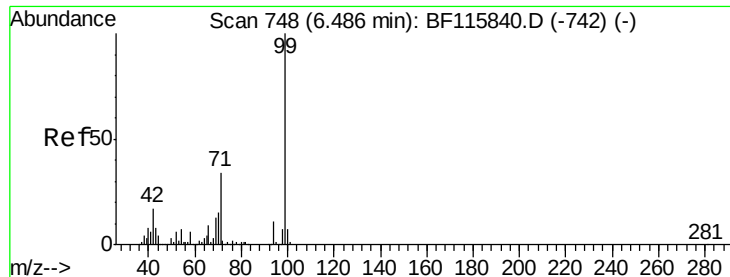

#7

Phenol-d6

Concen: 90.107 ng

RT: 6.49 min Scan# 748

Delta R.T. 0.00 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26

Instrument :

BNA_F

ClientSampled :

TP-11


Tot Ion: 99 Resp: 953083

Ion Ratio Lower Upper

99 100

42 16.7 13.8 20.6




71 33.8 27.1 40.7

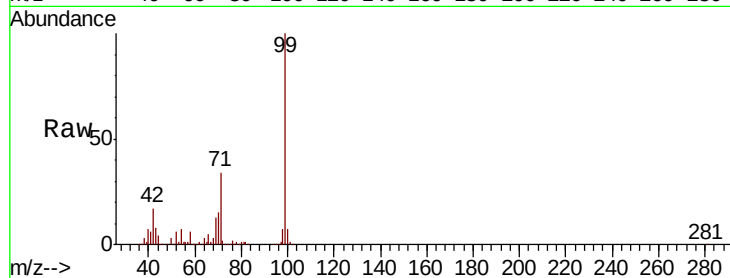

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

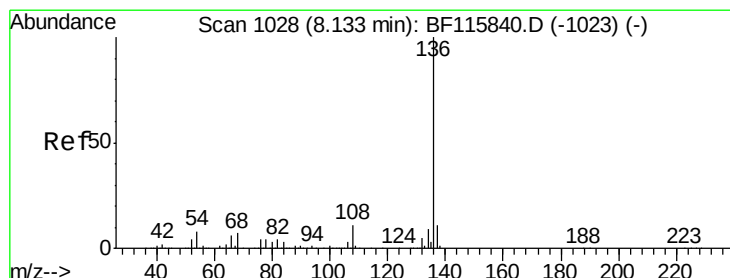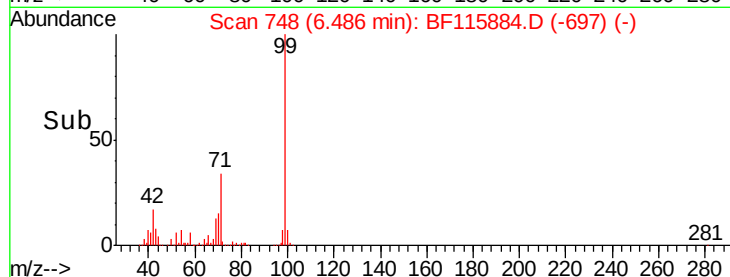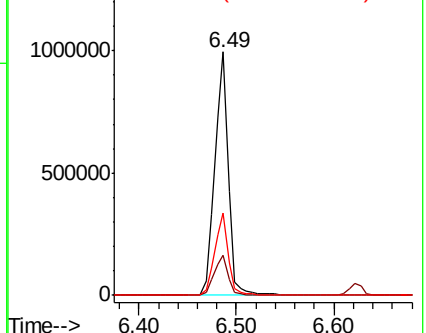

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.13 min Scan# 1028

Delta R.T. -0.00 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26

Tgt Ion: 136 Resp: 517234


Ion Ratio Lower Upper

136 100

137 11.3 9.1 13.7

54 7.0 6.1 9.1

68 5.7 5.4 8.2


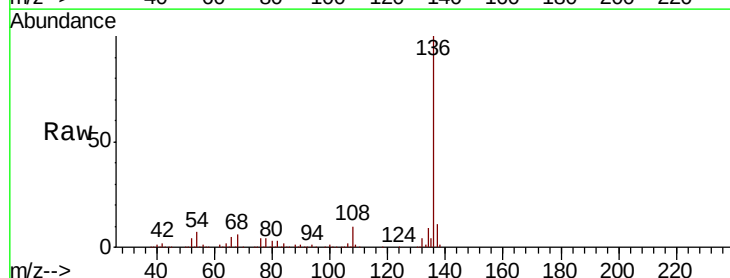



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

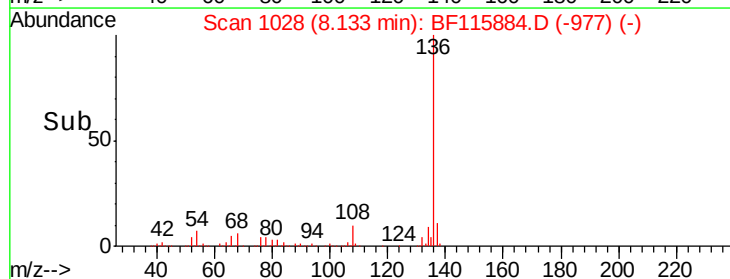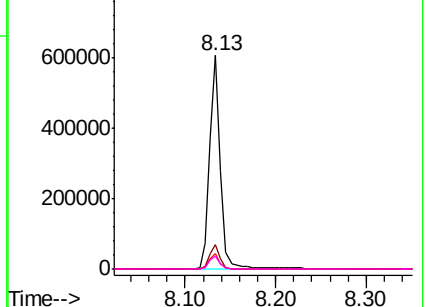


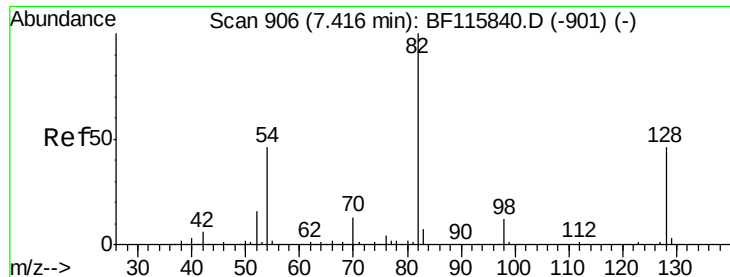




#23
 Nitrobenzene-d5
 Concen: 63.957 ng
 RT: 7.41 min Scan# 905
 Delta R.T. -0.01 min
 Lab File: BF115884.D
 Acq: 31 Jul 2019 23:26

Instrument :
 BNA_F
 ClientSampled :
 TP-11

Tot Ion: 82 Resp: 573091
 Ion Ratio Lower Upper
 82 100
 128 44.6 36.6 55.0
 54 45.8 36.6 55.0

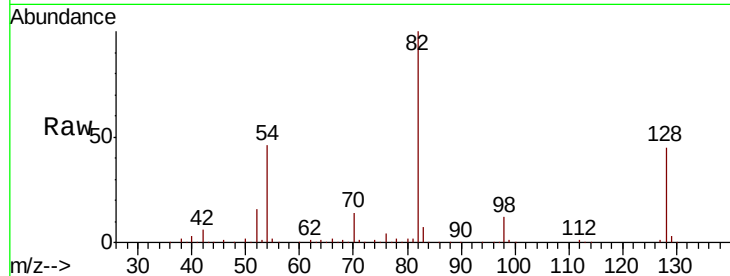


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

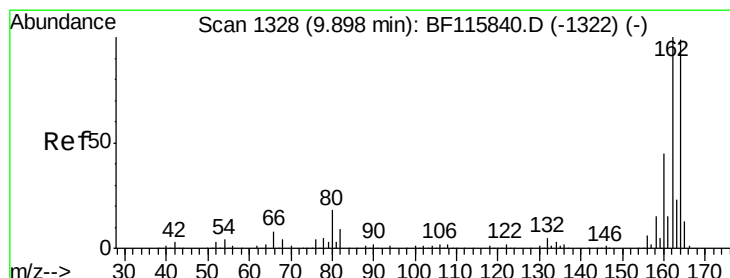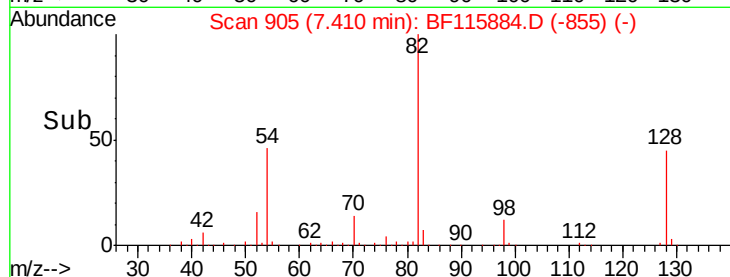
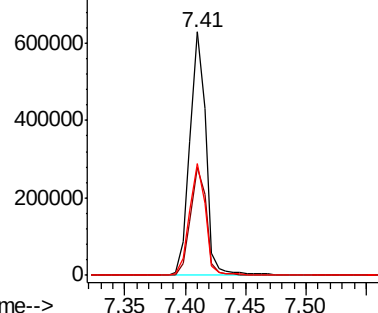



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.89 min Scan# 1327
 Delta R.T. -0.01 min
 Lab File: BF115884.D
 Acq: 31 Jul 2019 23:26

Tgt Ion: 164 Resp: 243146
 Ion Ratio Lower Upper
 164 100
 162 103.2 80.8 121.2
 160 46.4 36.2 54.4

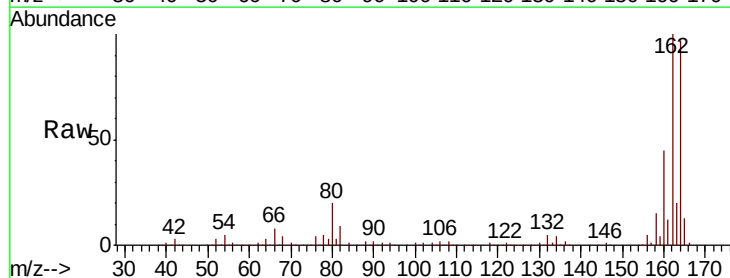

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

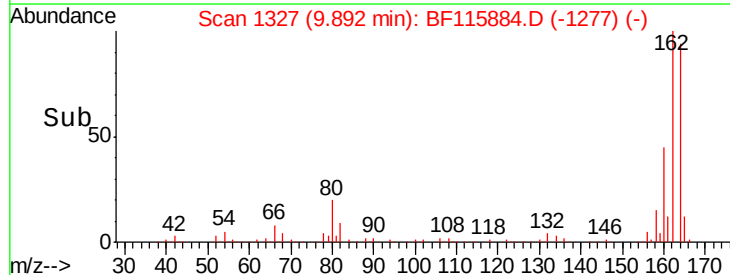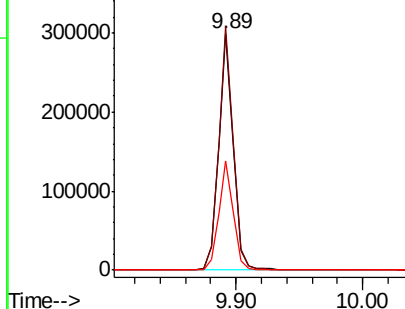

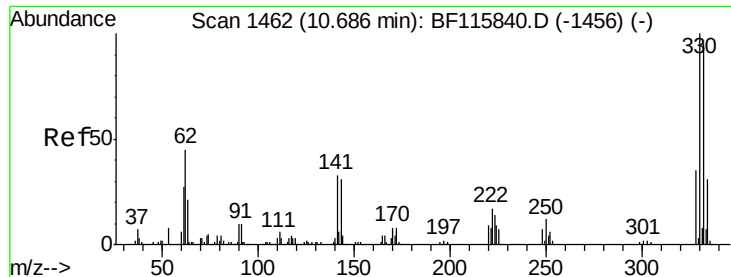

#42

2,4,6-Tribromophenol

Concen: 78.600 ng

RT: 10.68 min Scan# 1461

Delta R.T. -0.01 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26

Instrument :

BNA_F

ClientSampled :

TP-11


Tot Ion:330 Resp: 185290

Ion Ratio Lower Upper

330 100

332 96.2 77.7 116.5




141 34.7 28.1 42.1

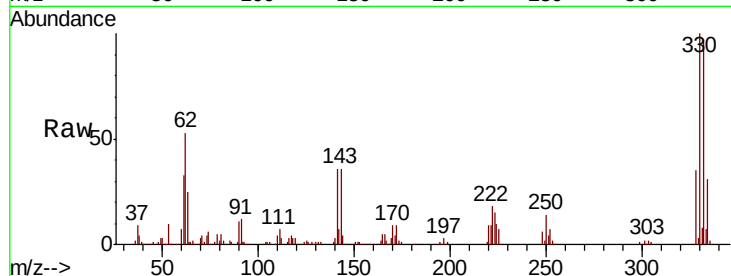

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

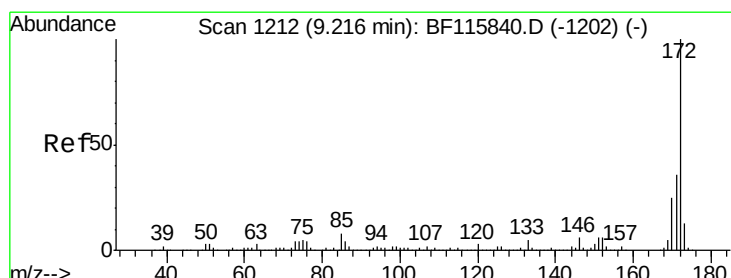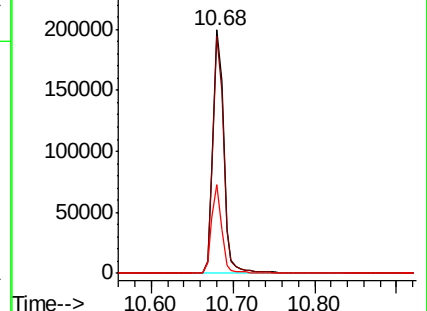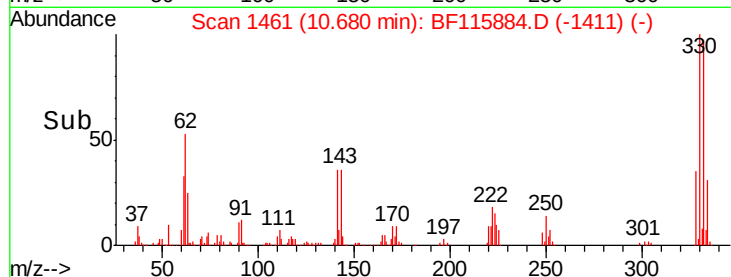

#45

2-Fluorobiphenyl

Concen: 74.952 ng

RT: 9.21 min Scan# 1211

Delta R.T. -0.01 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26


Tgt Ion:172 Resp: 972955

Ion Ratio Lower Upper

172 100

171 35.8 29.1 43.7



170 24.6 20.1 30.1

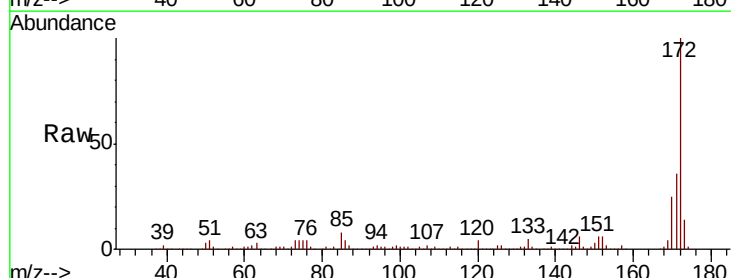


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

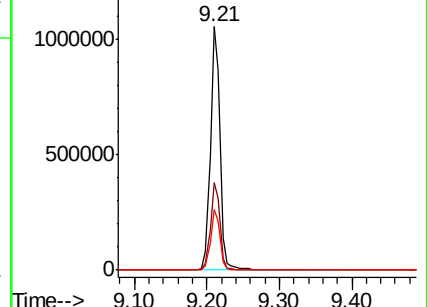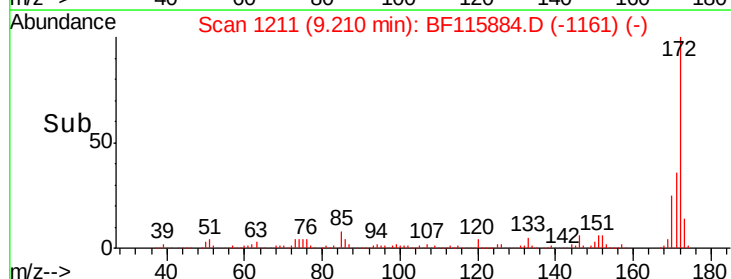


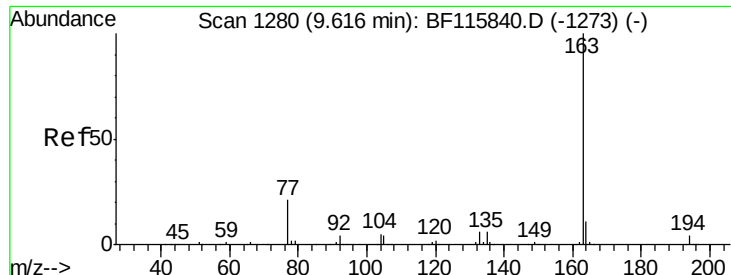




#50
Dimethylphthalate
Concen: 9.462 ng
RT: 9.60 min Scan# 1278
Delta R.T. -0.01 min
Lab File: BF115884.D
Acq: 31 Jul 2019 23:26

Instrument :
BNA_F
ClientSampleID :
TP-11

Tot Ion:163 Resp: 156644
Ion Ratio Lower Upper
163 100
194 3.6 3.0 4.6
164 9.9 8.4 12.6

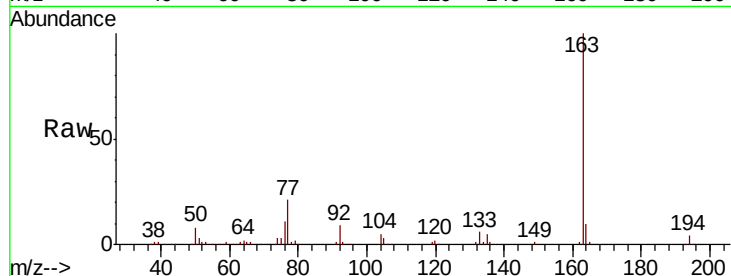


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

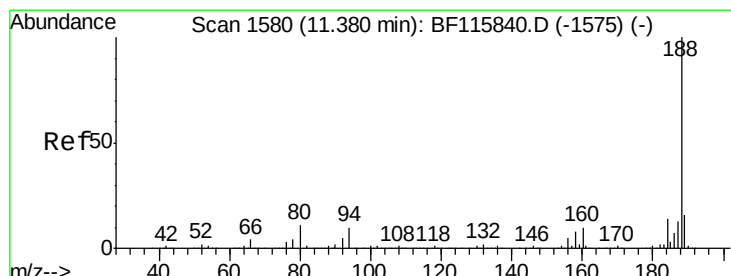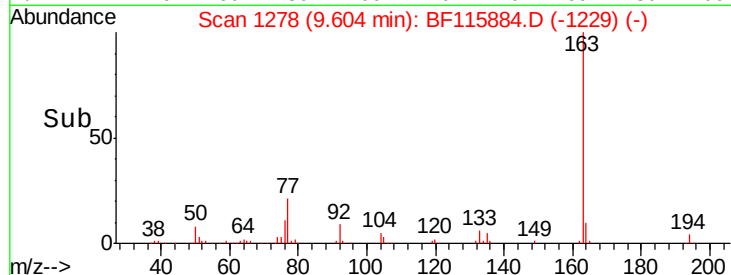
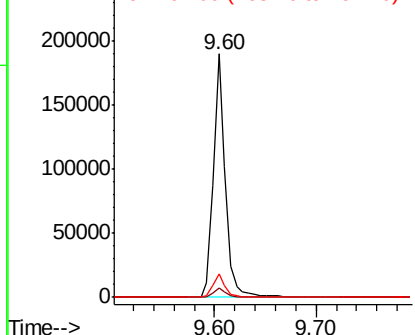



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.38 min Scan# 1580
Delta R.T. 0.00 min
Lab File: BF115884.D
Acq: 31 Jul 2019 23:26

Tgt Ion:188 Resp: 367354
Ion Ratio Lower Upper
188 100
94 9.3 8.0 12.0
80 9.7 8.6 12.8

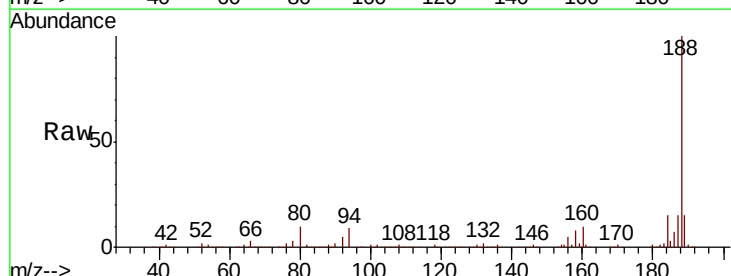

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

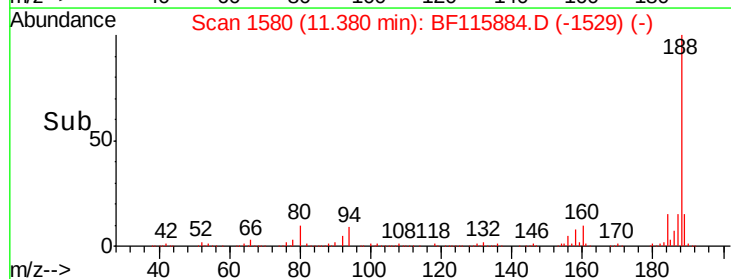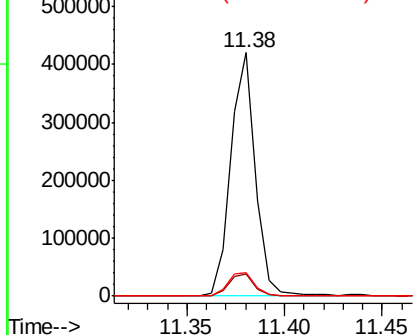

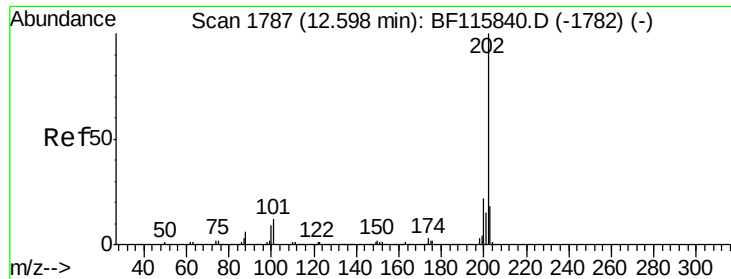

#75

Fluoranthene

Concen: 2.072 ng

RT: 12.59 min Scan# 1786

Delta R.T. -0.01 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26

Instrument :

BNA_F

ClientSampleId :

TP-11


Tot Ion:202 Resp: 40746

Ion Ratio Lower Upper

202 100

101 11.2 0.0 31.5




203 17.1 0.0 37.9

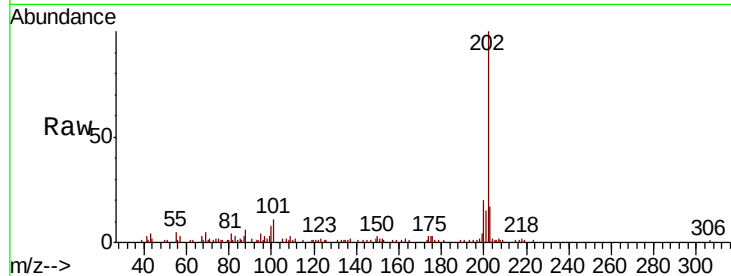

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

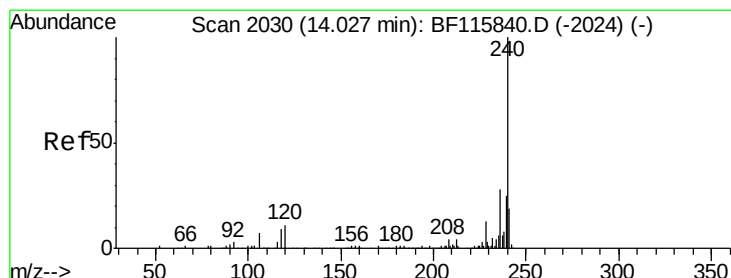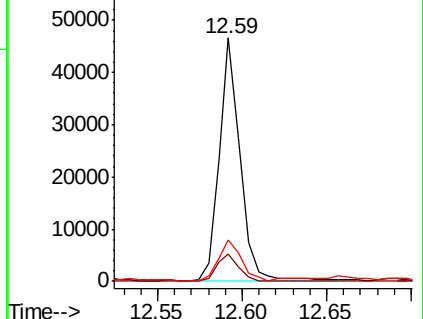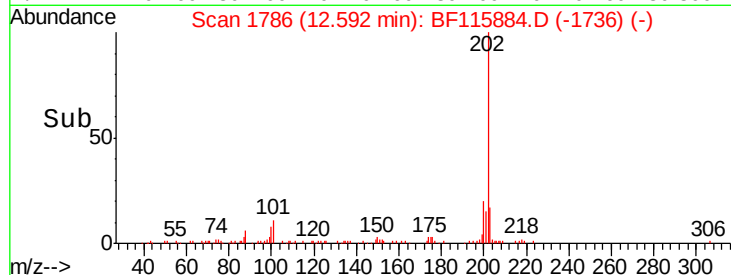

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.02 min Scan# 2029

Delta R.T. -0.01 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26


Tgt Ion:240 Resp: 332303

Ion Ratio Lower Upper

240 100

120 11.1 8.5 12.7



236 27.1 22.2 33.2

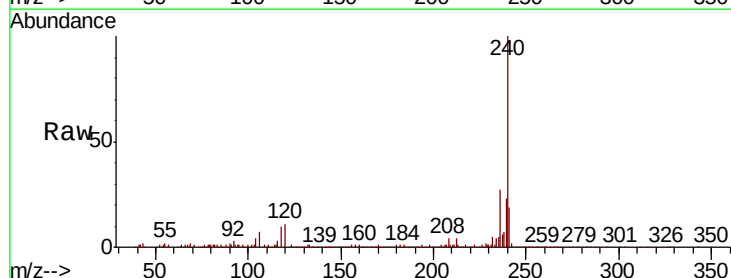


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

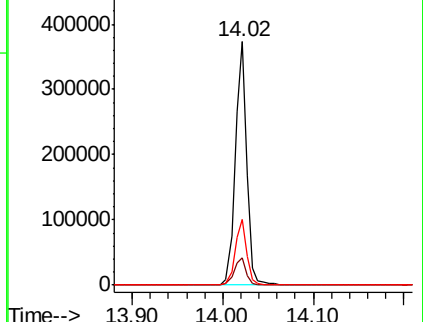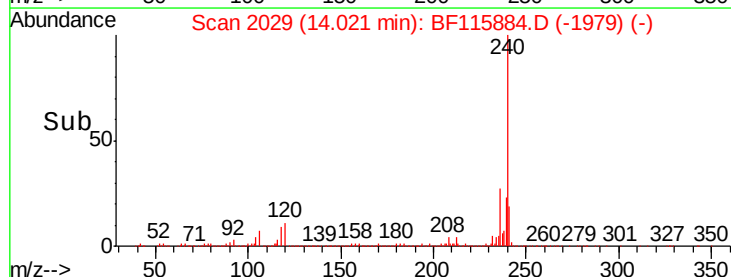

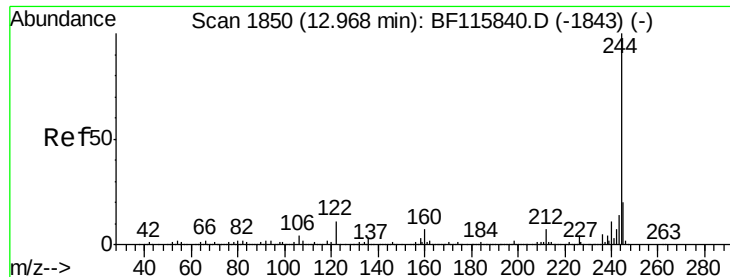

#79

Terphenyl-d14

Concen: 54.397 ng

RT: 12.96 min Scan# 1849

Delta R.T. -0.01 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26

Instrument :

BNA_F

ClientSampleId :

TP-11


Tot Ion:244 Resp: 857849

Ion Ratio Lower Upper

244 100

212 6.9 5.6 8.4




122 12.0 8.6 13.0

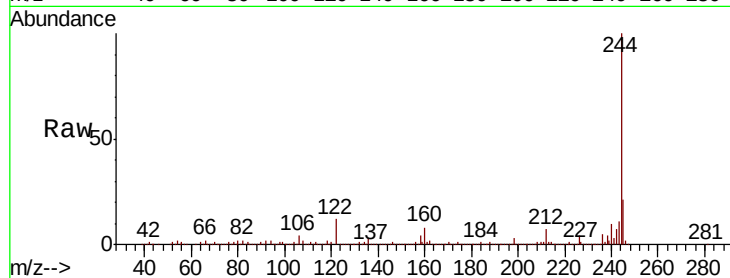

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

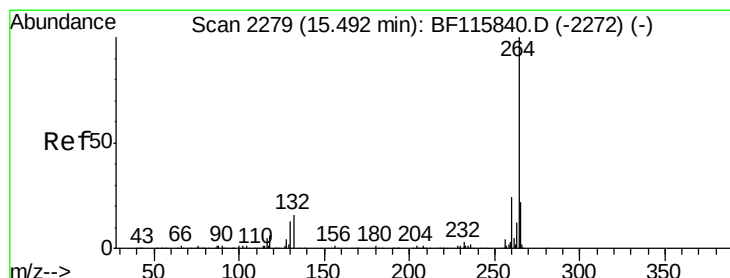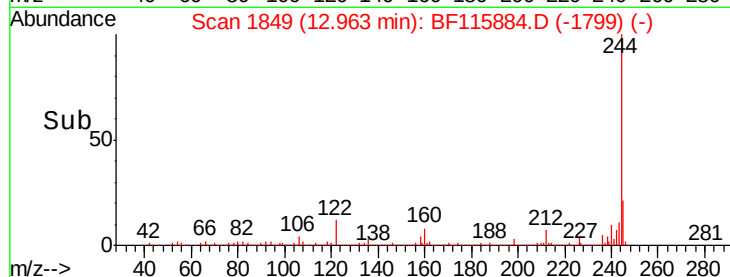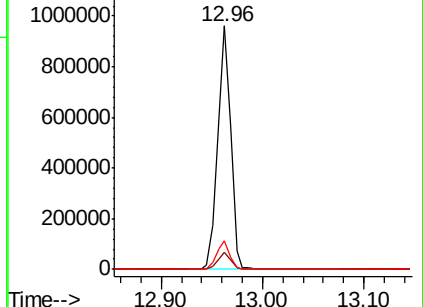

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.49 min Scan# 2279

Delta R.T. 0.00 min

Lab File: BF115884.D

Acq: 31 Jul 2019 23:26


Tgt Ion:264 Resp: 325765

Ion Ratio Lower Upper

264 100

260 24.4 19.4 29.2

265 22.2 17.5 26.3

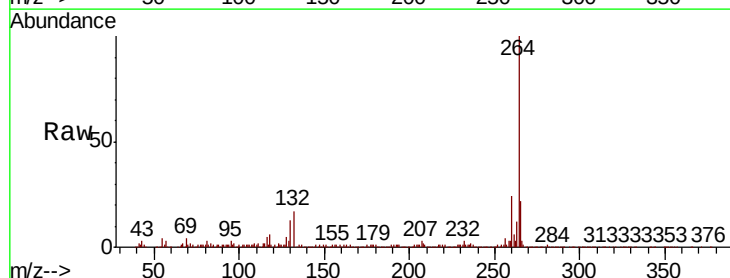

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

