


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073119\
 Data File : BF115853.D
 Acq On : 31 Jul 2019 7:33
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 15:31:51 2019

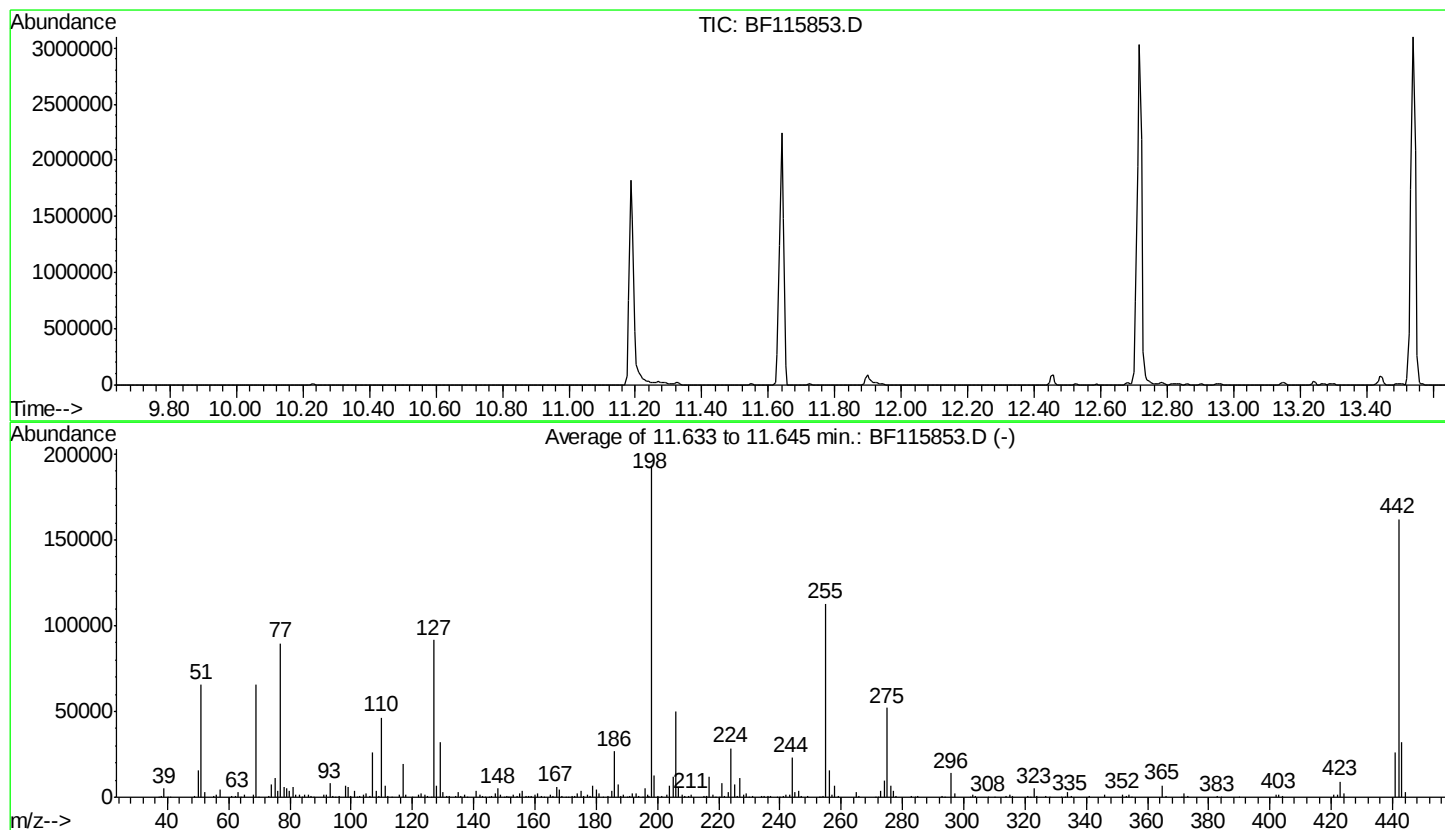

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	65410	PASS
68	69	0.00	2	1.8	1183	PASS
69	198	0.00	100	34.1	65826	PASS
70	69	0.00	2	0.5	346	PASS
127	198	10	80	47.4	91645	PASS
197	198	0.00	2	0.6	1175	PASS
198	198	100	100	100.0	193258	PASS
199	198	5	9	6.6	12840	PASS
275	198	10	60	27.0	52200	PASS
365	198	1	100	3.7	7084	PASS
441	198	0.01	100	13.4	25817	PASS
442	198	50	100	83.9	162114	PASS
443	442	15	24	19.8	32051	PASS