


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF073119\
 Data File : BF115869.D
 Acq On : 31 Jul 2019 16:42
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 15:31:51 2019

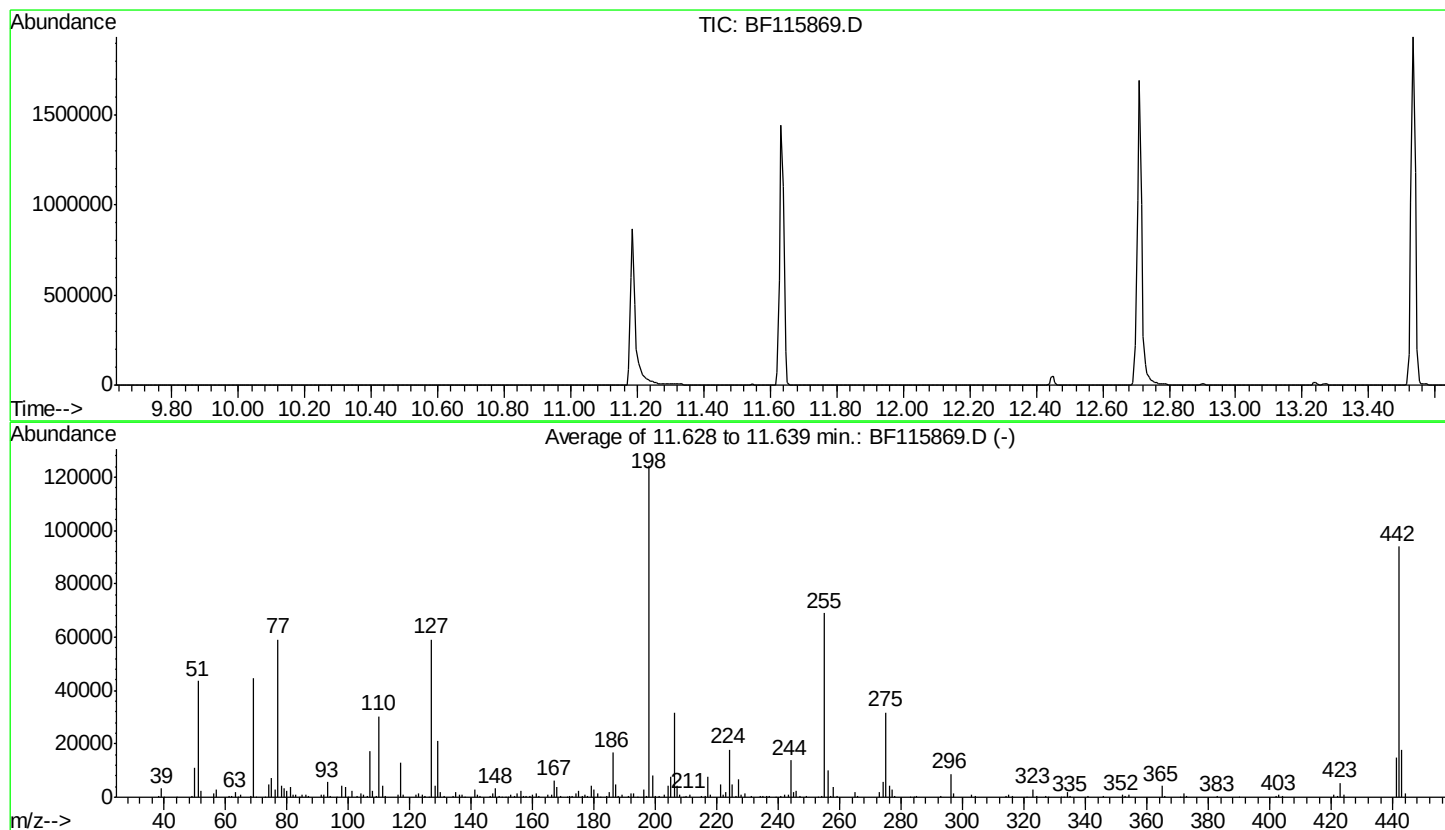

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	43629	PASS
68	69	0.00	2	1.5	656	PASS
69	198	0.00	100	36.0	44768	PASS
70	69	0.00	2	0.3	138	PASS
127	198	10	80	47.6	59136	PASS
197	198	0.00	2	0.5	605	PASS
198	198	100	100	100.0	124314	PASS
199	198	5	9	6.7	8372	PASS
275	198	10	60	25.5	31761	PASS
365	198	1	100	3.4	4236	PASS
441	198	0.01	100	11.9	14814	PASS
442	198	50	100	75.5	93864	PASS
443	442	15	24	19.2	17997	PASS