
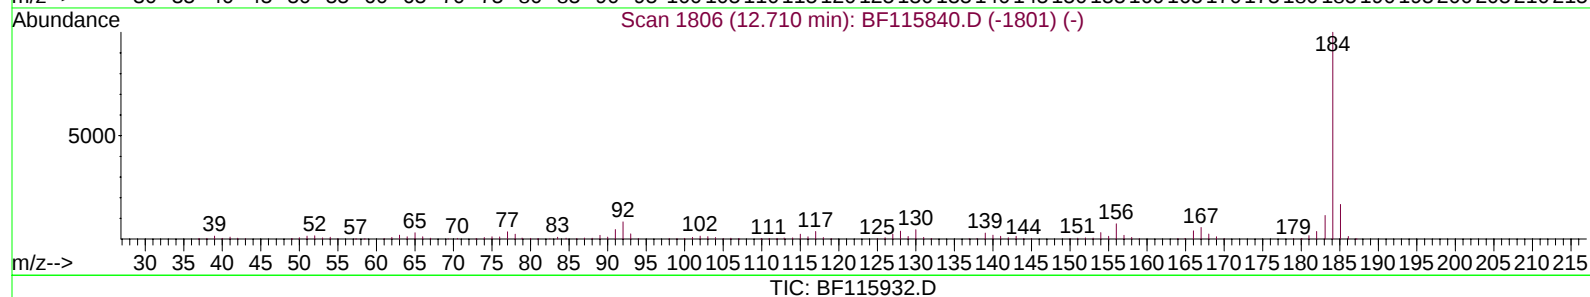
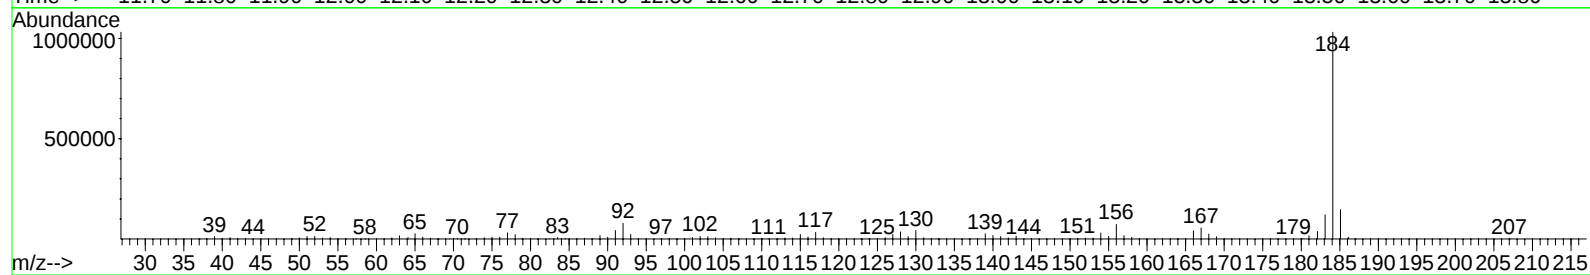


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080219\
Data File : BF115932.D
Acq On : 2 Aug 2019 8:10
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:46:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

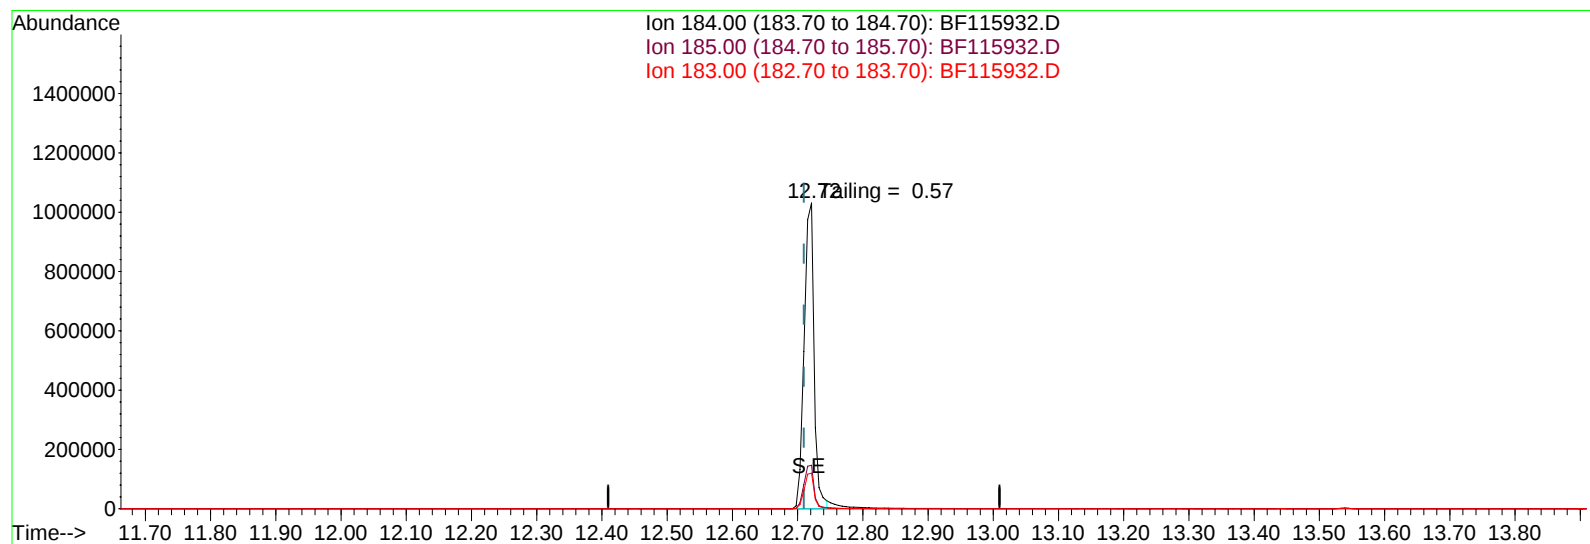

(77) Benzidine




12.721min (+0.012) 221557.93ng

response 1130259

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.26
183.00	11.40	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080219\
 Data File : BF115932.D
 Acq On : 2 Aug 2019 8:10
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:46:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:31:51 2019
 Response via : Initial Calibration

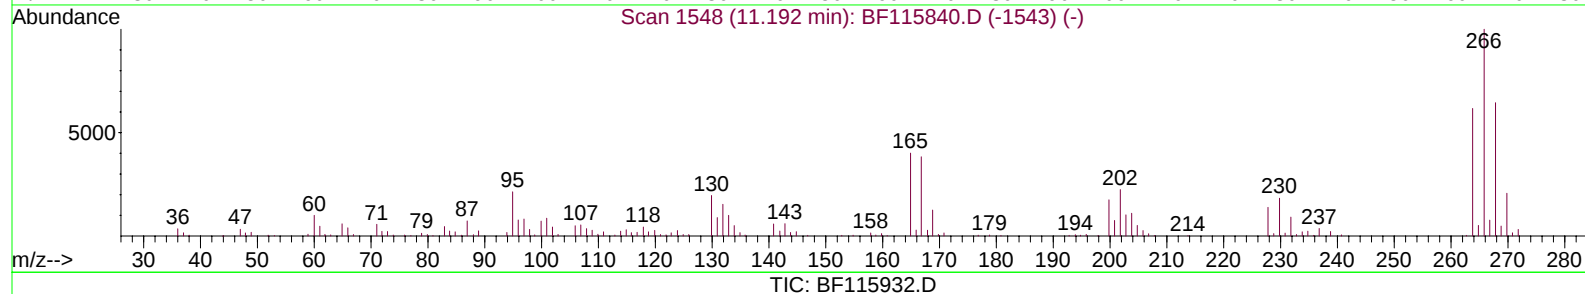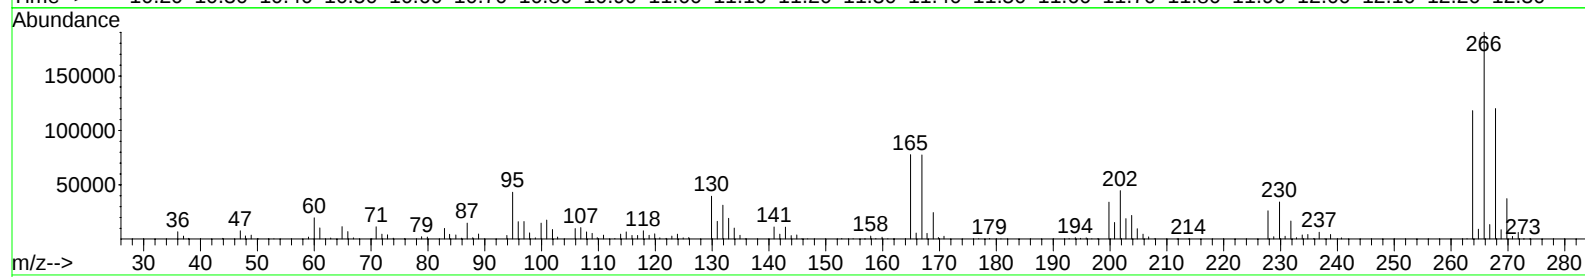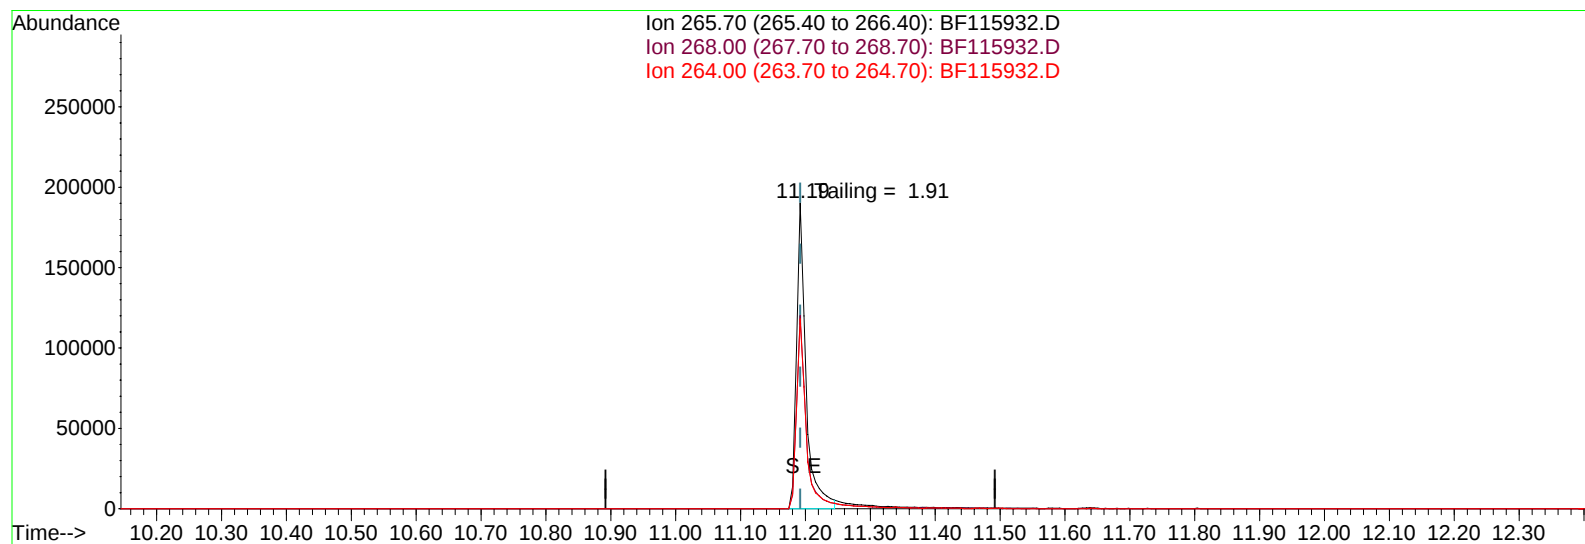

(70) Pentachlorophenol (C)

11.192min (-0.000) 325678.93ng

response 211384

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.15
264.00	61.70	62.14
0.00	0.00	0.00