
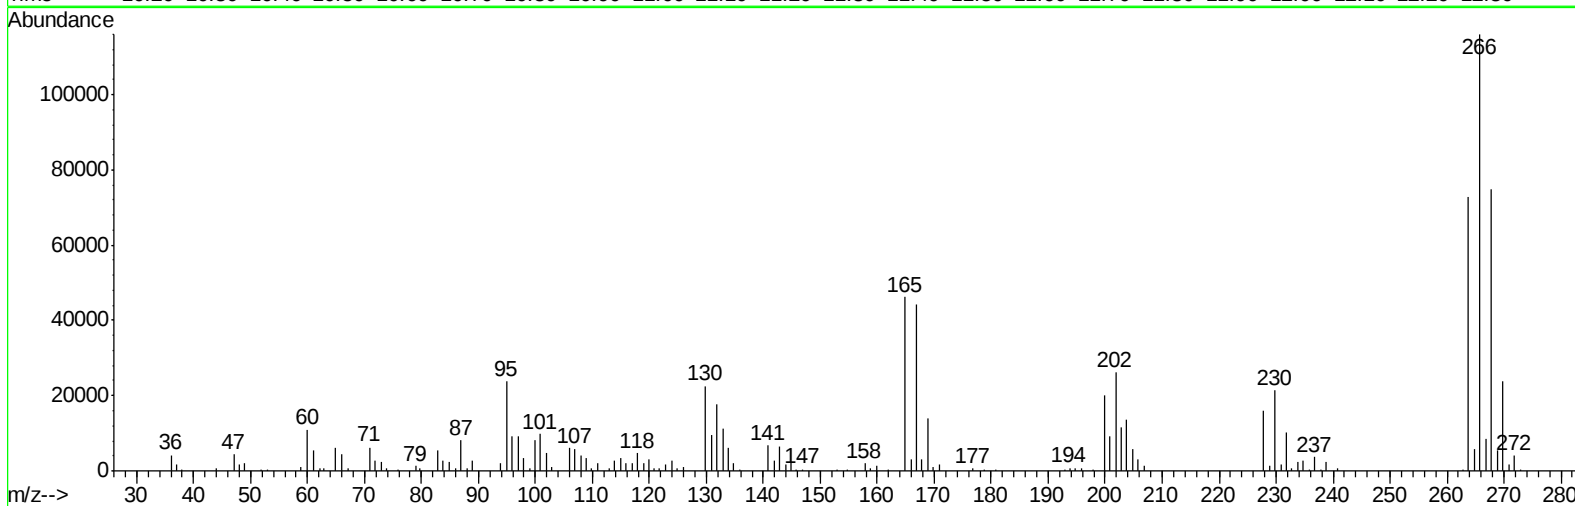


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080219\
Data File : BF115947.D
Acq On : 2 Aug 2019 15:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 07:05:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

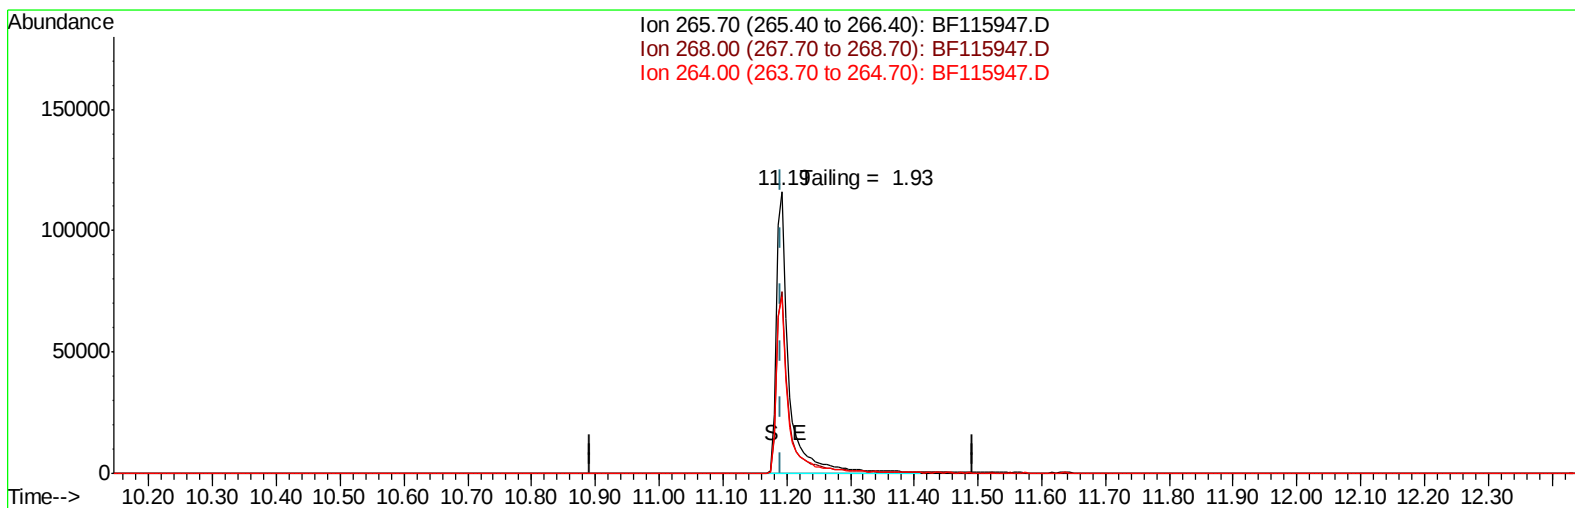

TIC: BF115947.D

(70) Pentachlorophenol (C)



11.192min (-0.000) 41228.57ng

response 162788

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.58
264.00	61.70	62.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080219\
Data File : BF115947.D
Acq On : 2 Aug 2019 15:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 07:05:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

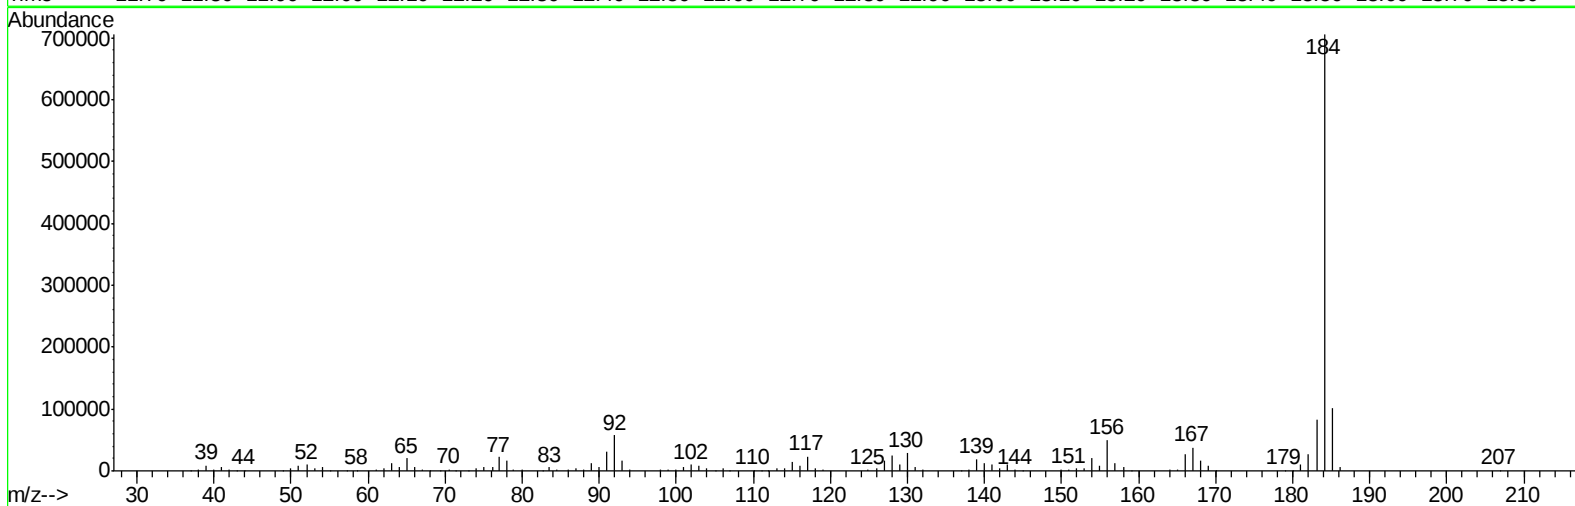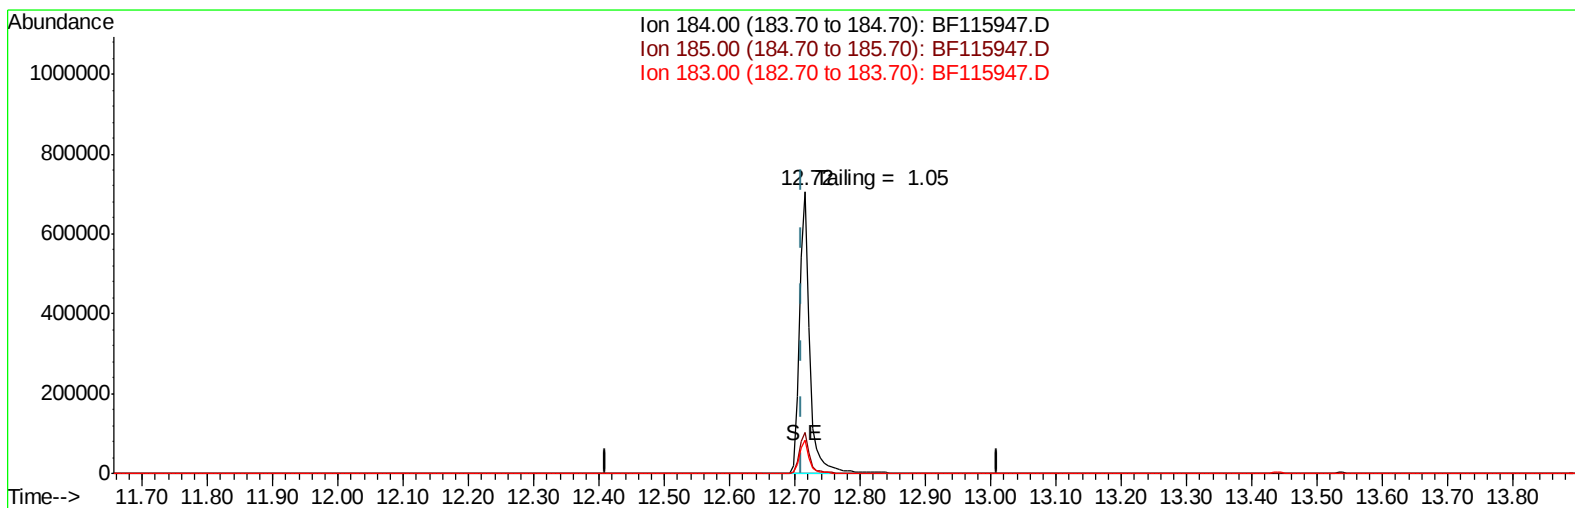

TIC: BF115947.D

(77) Benzidine

12.715min (+0.006) 0.00ng

response 769691

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.34
183.00	11.40	11.89
0.00	0.00	0.00