


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080219\
Data File : BF115932.D
Acq On : 2 Aug 2019 8:10
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 07 11:13:18 2019

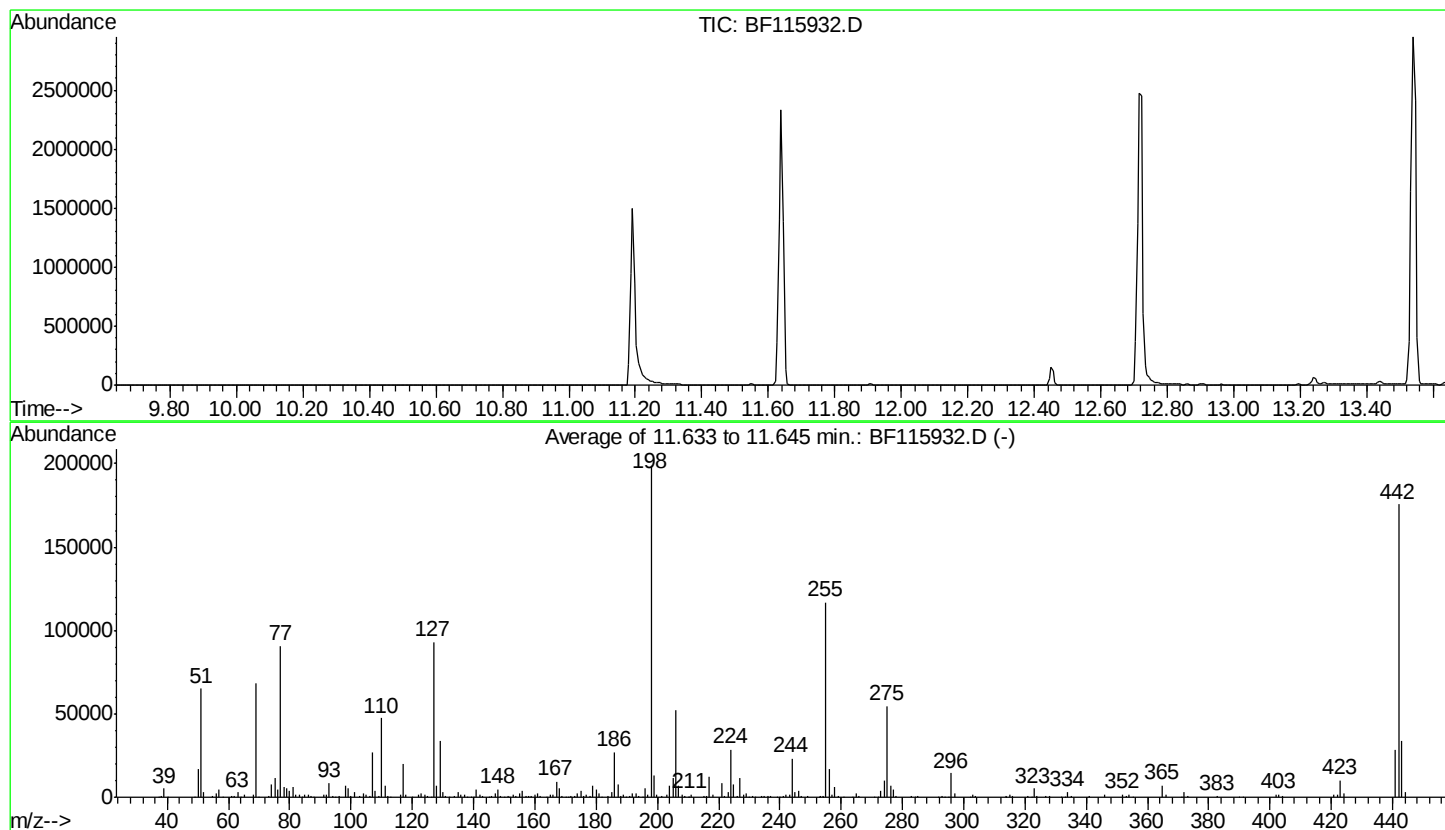

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	65194	PASS
68	69	0.00	2	1.7	1200	PASS
69	198	0.00	100	34.5	68645	PASS
70	69	0.00	2	0.5	343	PASS
127	198	10	80	46.7	92882	PASS
197	198	0.00	2	0.6	1242	PASS
198	198	100	100	100.0	198805	PASS
199	198	5	9	6.6	13142	PASS
275	198	10	60	27.6	54842	PASS
365	198	1	100	3.6	7249	PASS
441	198	0.01	100	14.1	28099	PASS
442	198	50	100	88.2	175429	PASS
443	442	15	24	19.2	33763	PASS