
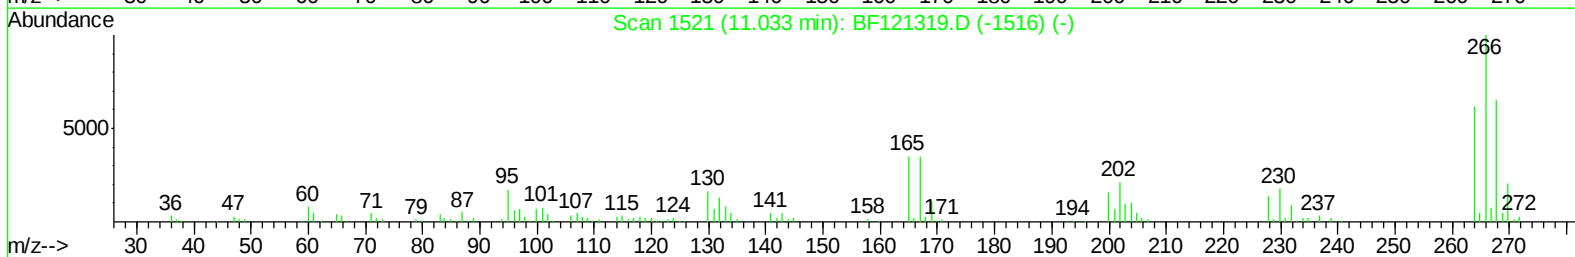
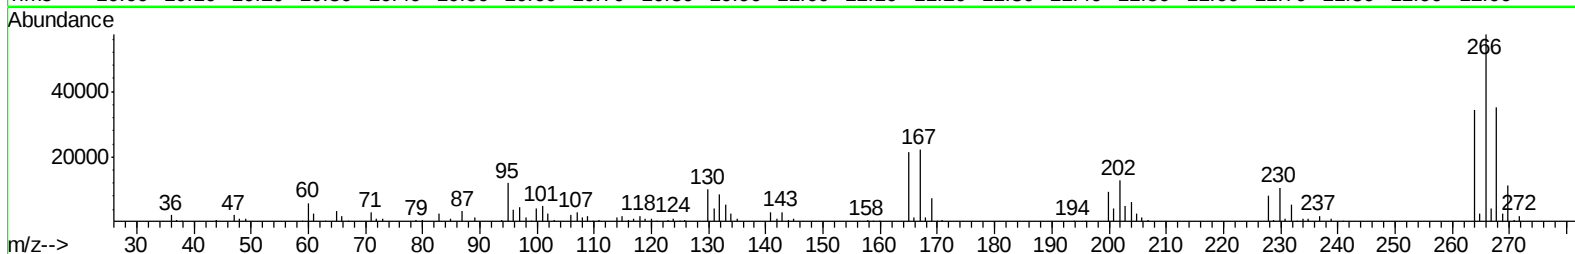


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081820\
 Data File : BF121315.D
 Acq On : 18 Aug 2020 9:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:57:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 18 15:43:38 2020
 Response via : Initial Calibration

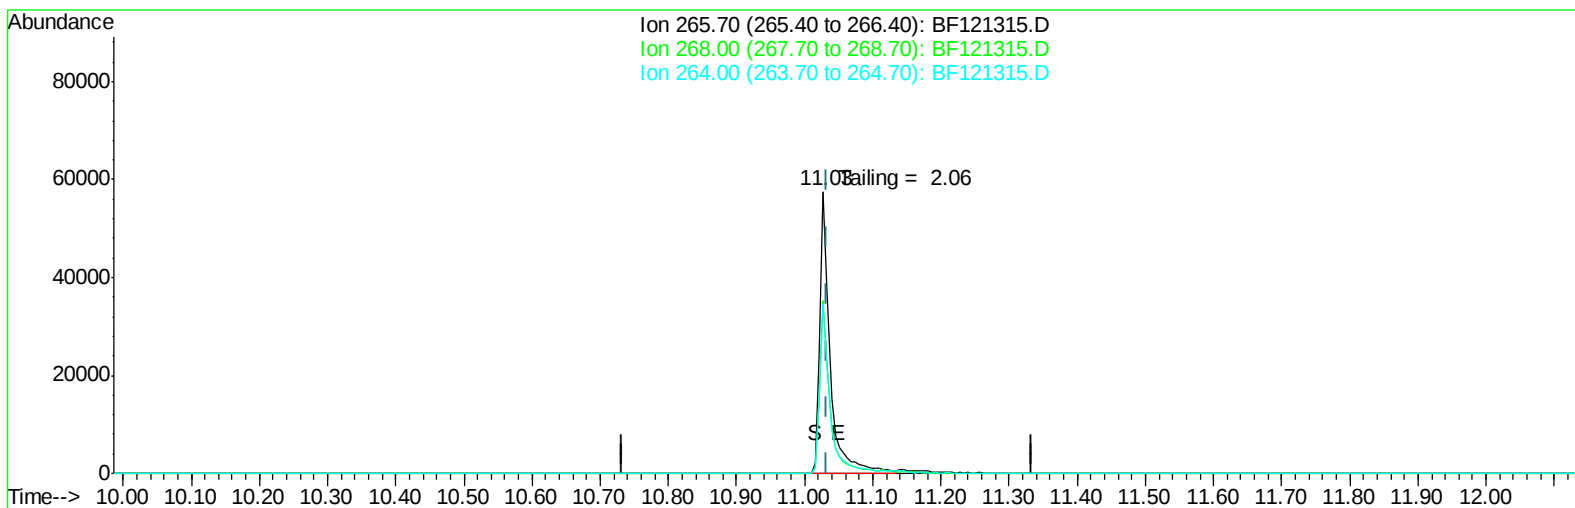

TIC: BF121315.D

(70) Pentachlorophenol (C)




11.027min (-0.006) 14694.26ng

response 60965

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	61.28
264.00	61.60	59.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081820\
Data File : BF121315.D
Acq On : 18 Aug 2020 9:30
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:57:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 18 15:43:38 2020
Response via : Initial Calibration

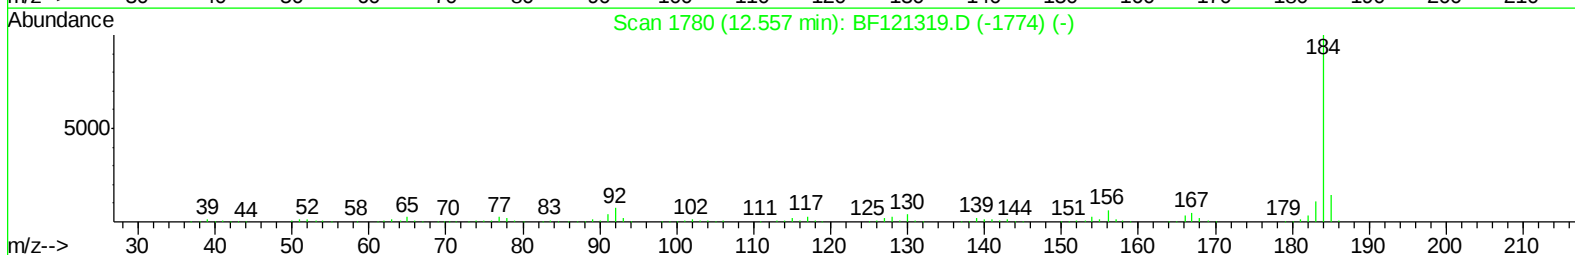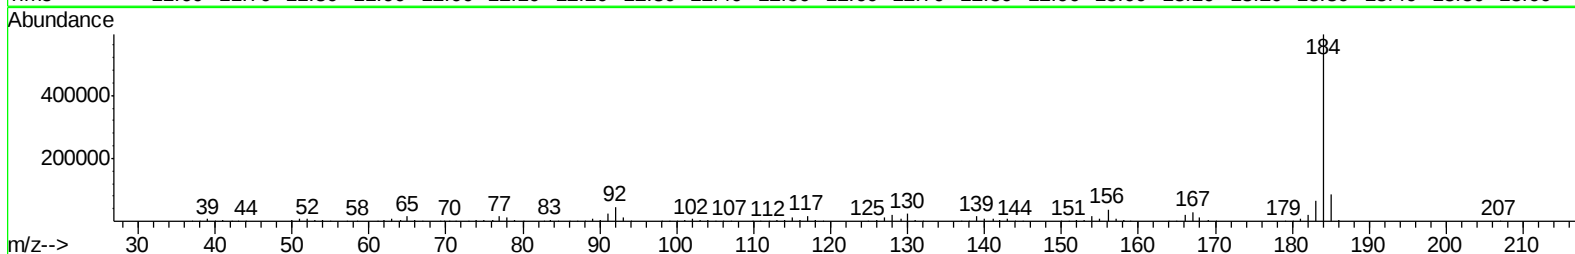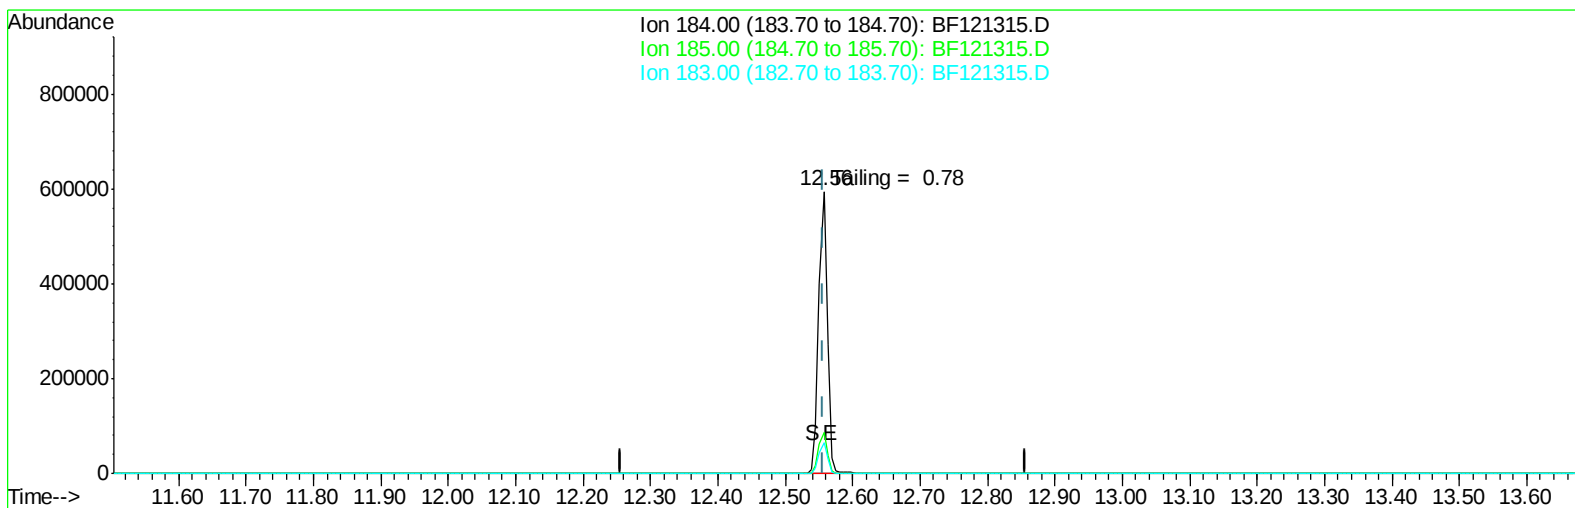

TIC: BF121315.D

(77) Benzidine

12.557min (-0.000) 6943.07ng

response 503361

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.68
183.00	10.80	10.96
0.00	0.00	0.00