


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081820\
 Data File : BF121315.D
 Acq On : 18 Aug 2020 9:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 18 15:43:38 2020

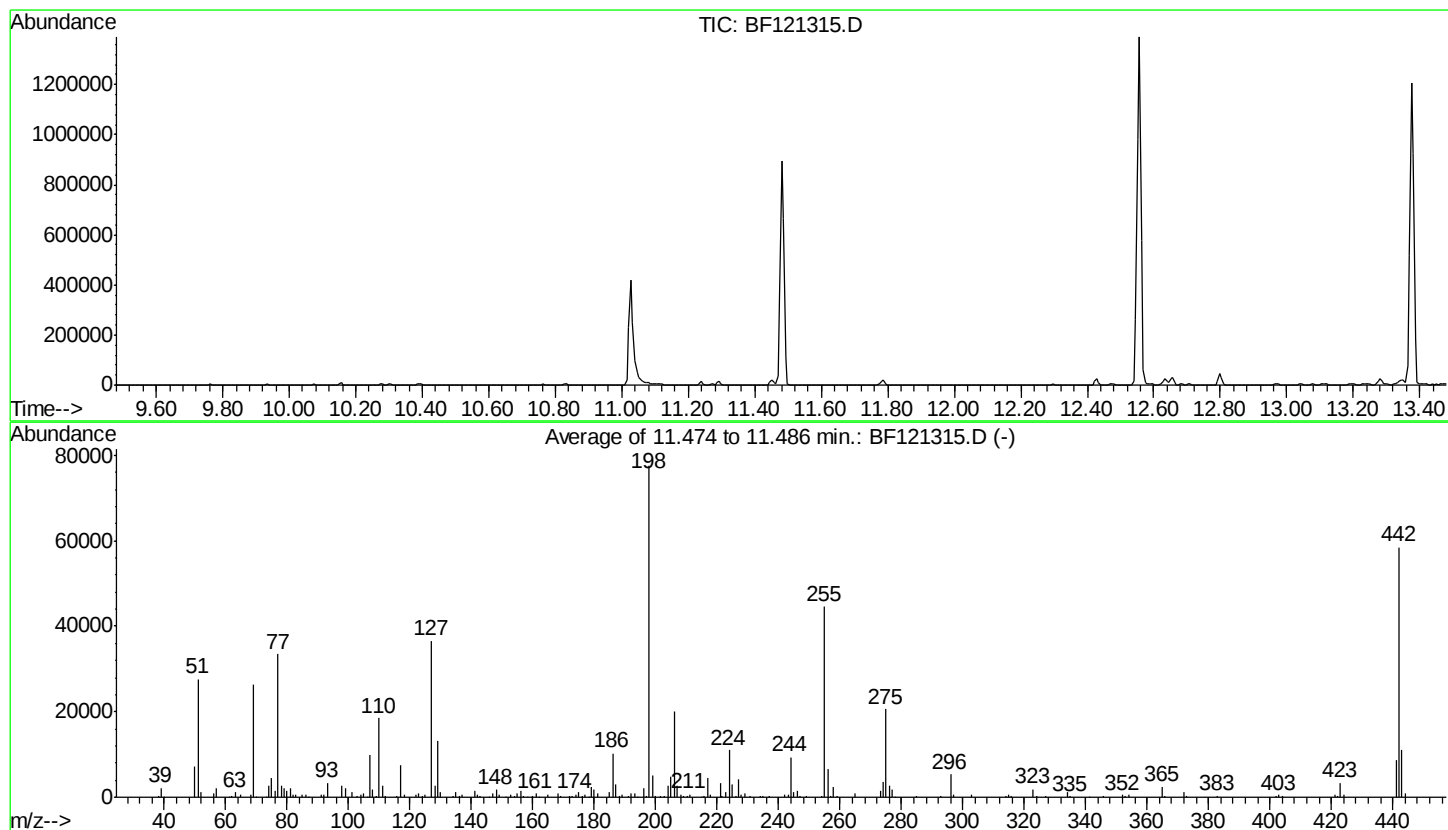

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	27682	PASS
68	69	0.00	2	1.9	509	PASS
69	198	0.00	100	33.9	26309	PASS
70	69	0.00	2	0.4	104	PASS
127	198	10	80	47.1	36552	PASS
197	198	0.00	2	0.5	406	PASS
198	198	100	100	100.0	77573	PASS
199	198	5	9	6.7	5219	PASS
275	198	10	60	26.5	20568	PASS
365	198	1	100	3.3	2555	PASS
441	198	0.01	100	11.3	8738	PASS
442	198	50	100	75.5	58537	PASS
443	442	15	24	18.8	10997	PASS