
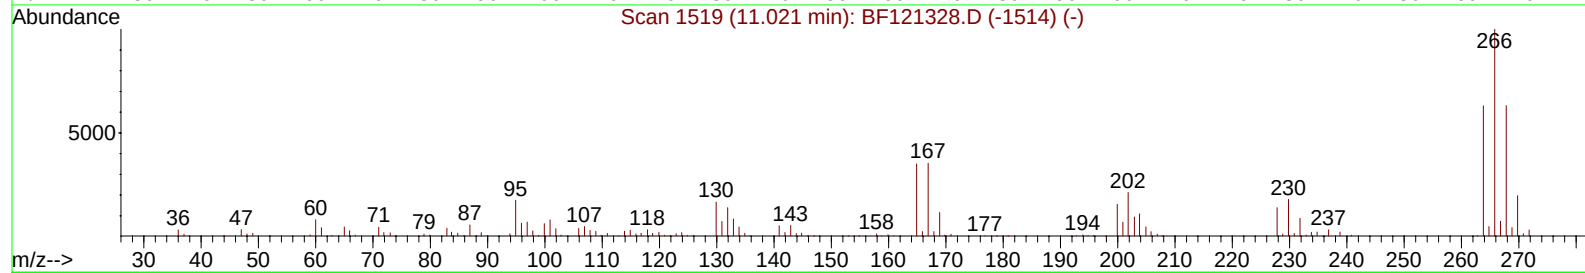
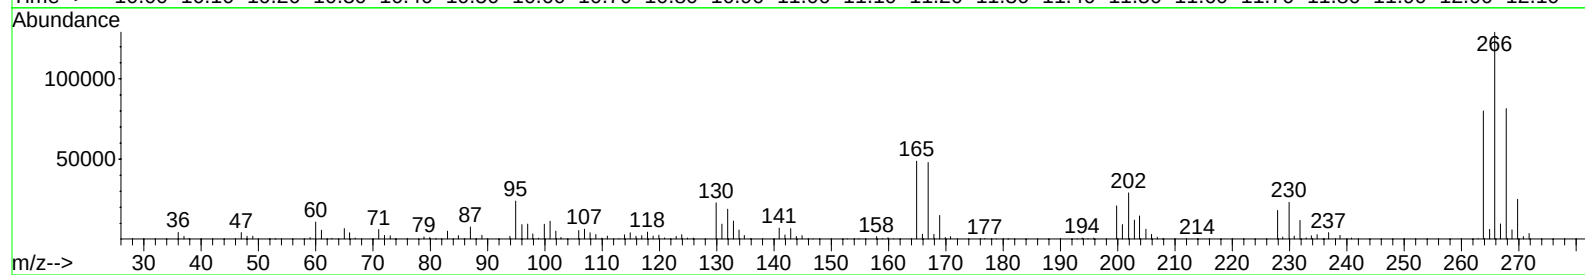


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082020\
 Data File : BF121334.D
 Acq On : 20 Aug 2020 7:52
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 18:57:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration

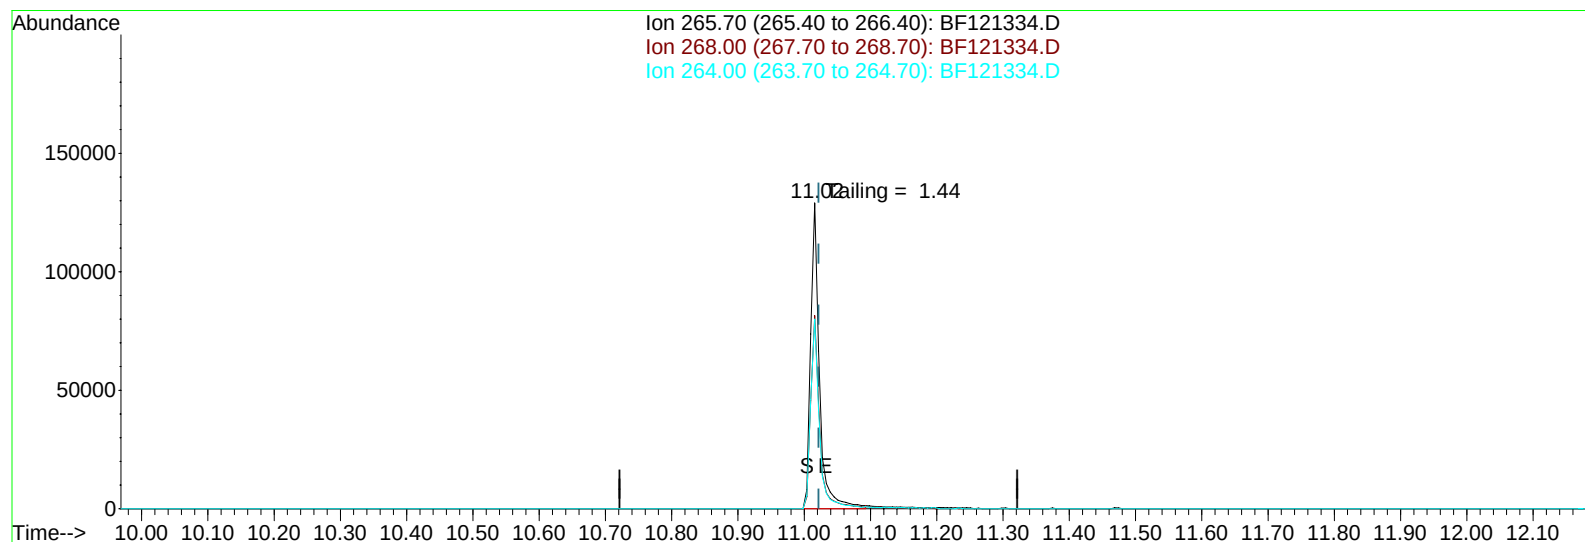

TIC: BF121334.D

(70) Pentachlorophenol (C)




11.016min (-0.006) 96599.38ng

response 123650

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.15
264.00	63.10	61.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082020\
 Data File : BF121334.D
 Acq On : 20 Aug 2020 7:52
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 18:57:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration

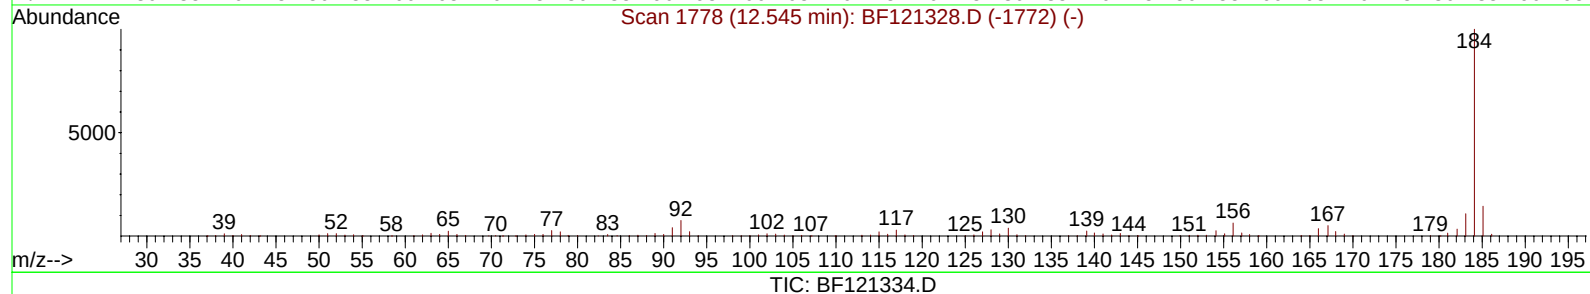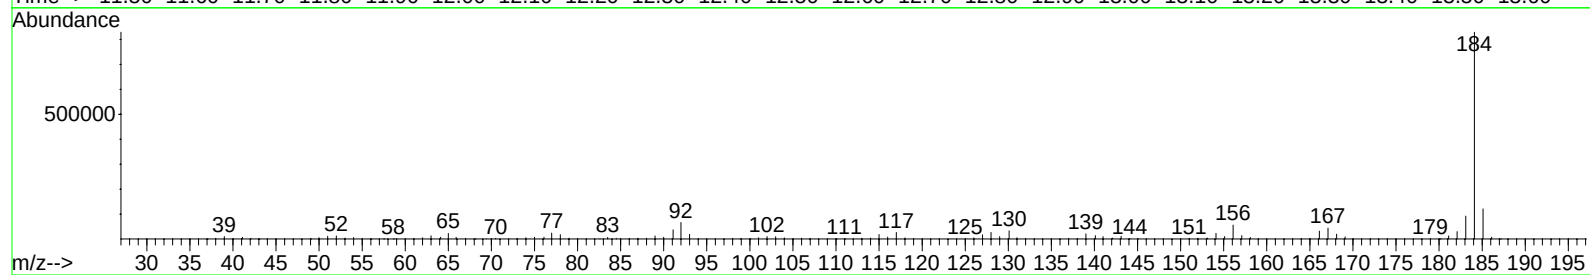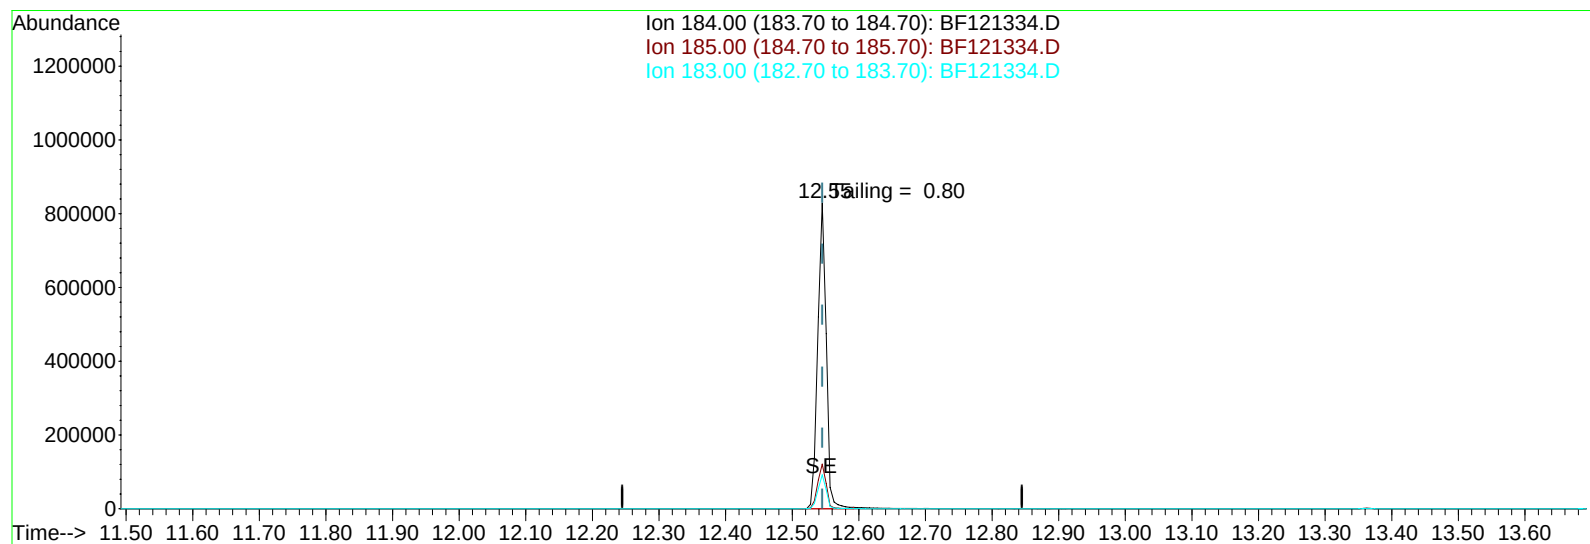

(77) Benzidine

12.545min (+0.000) 11079.89ng

response 744525

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.62
183.00	10.90	11.12
0.00	0.00	0.00