



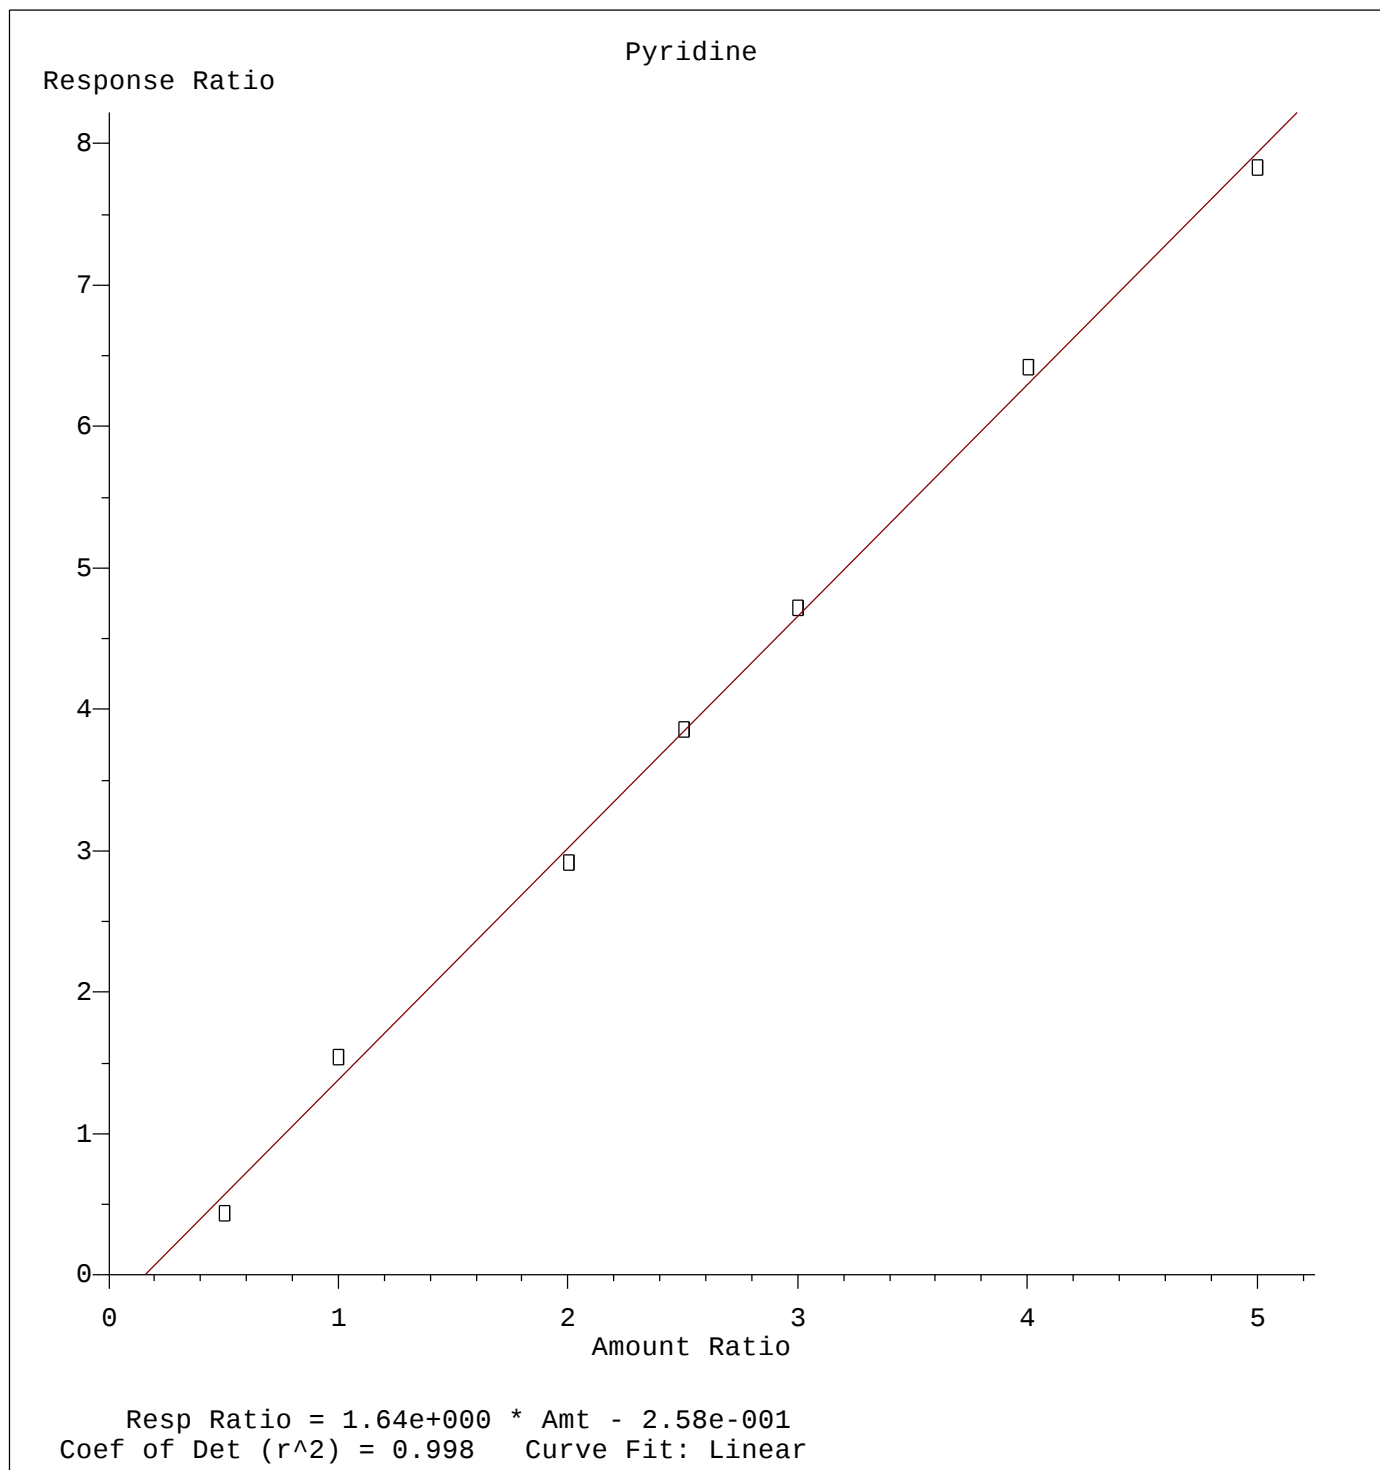

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
Calibration Table Last Updated: Wed Aug 28 13:34:15 2019


n-Nitrosodimethylamine

Response Ratio

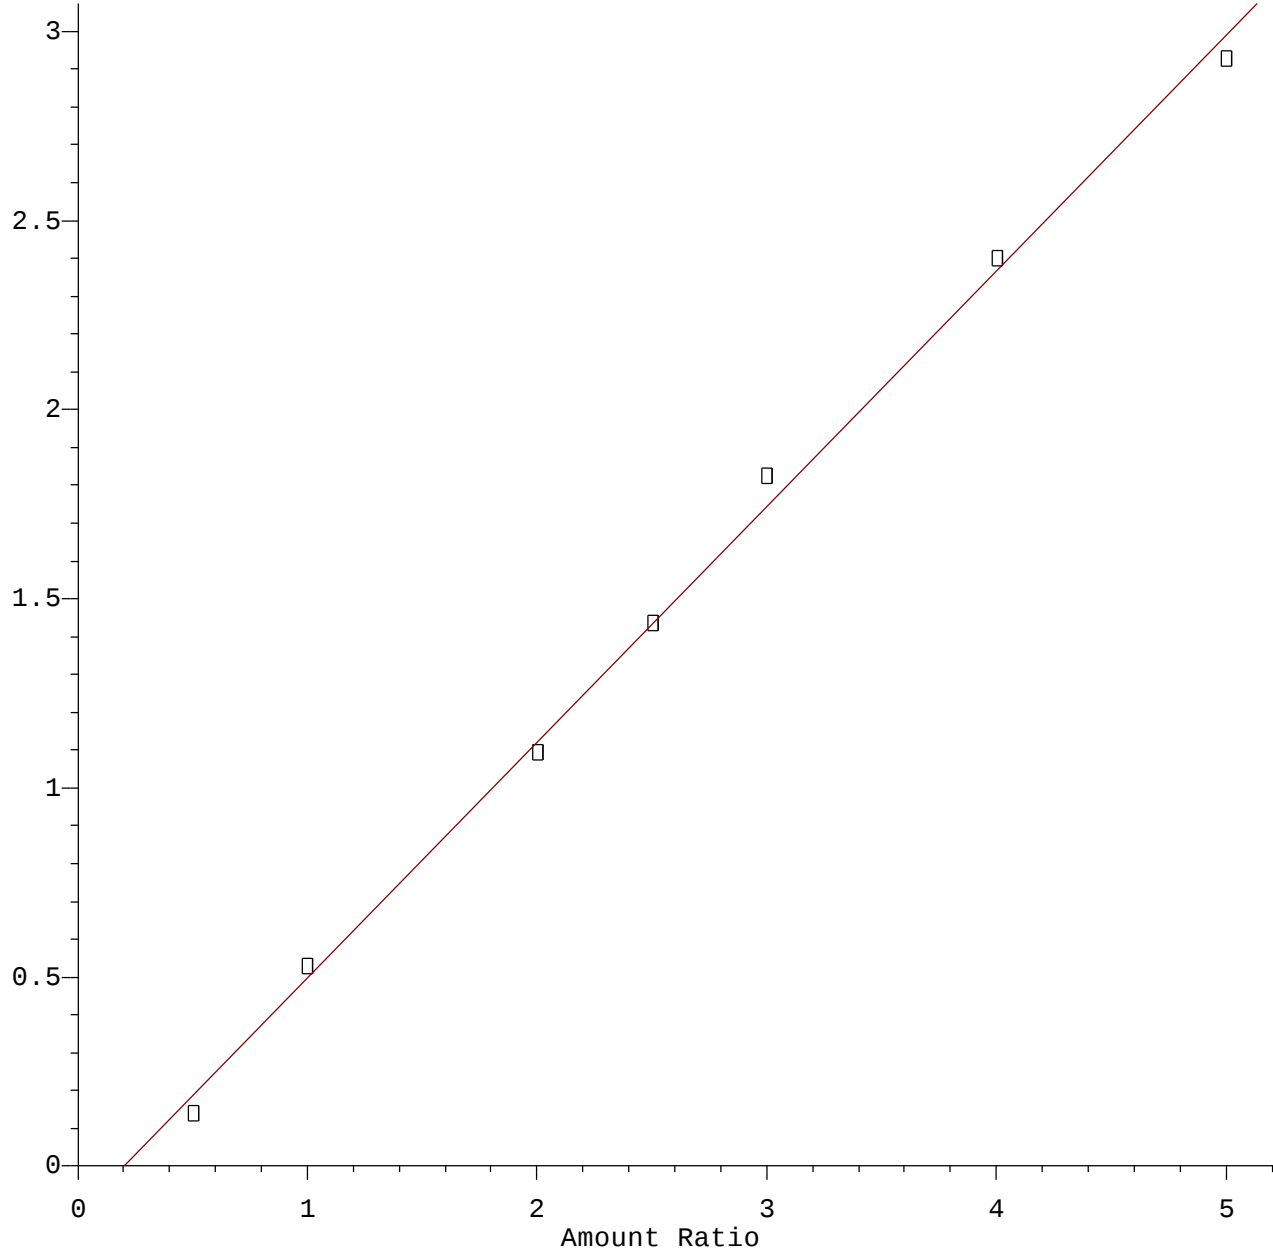

Resp Ratio = $6.23 \times 10^{-1} \times \text{Amt} - 1.24 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
Calibration Table Last Updated: Wed Aug 28 13:34:15 2019

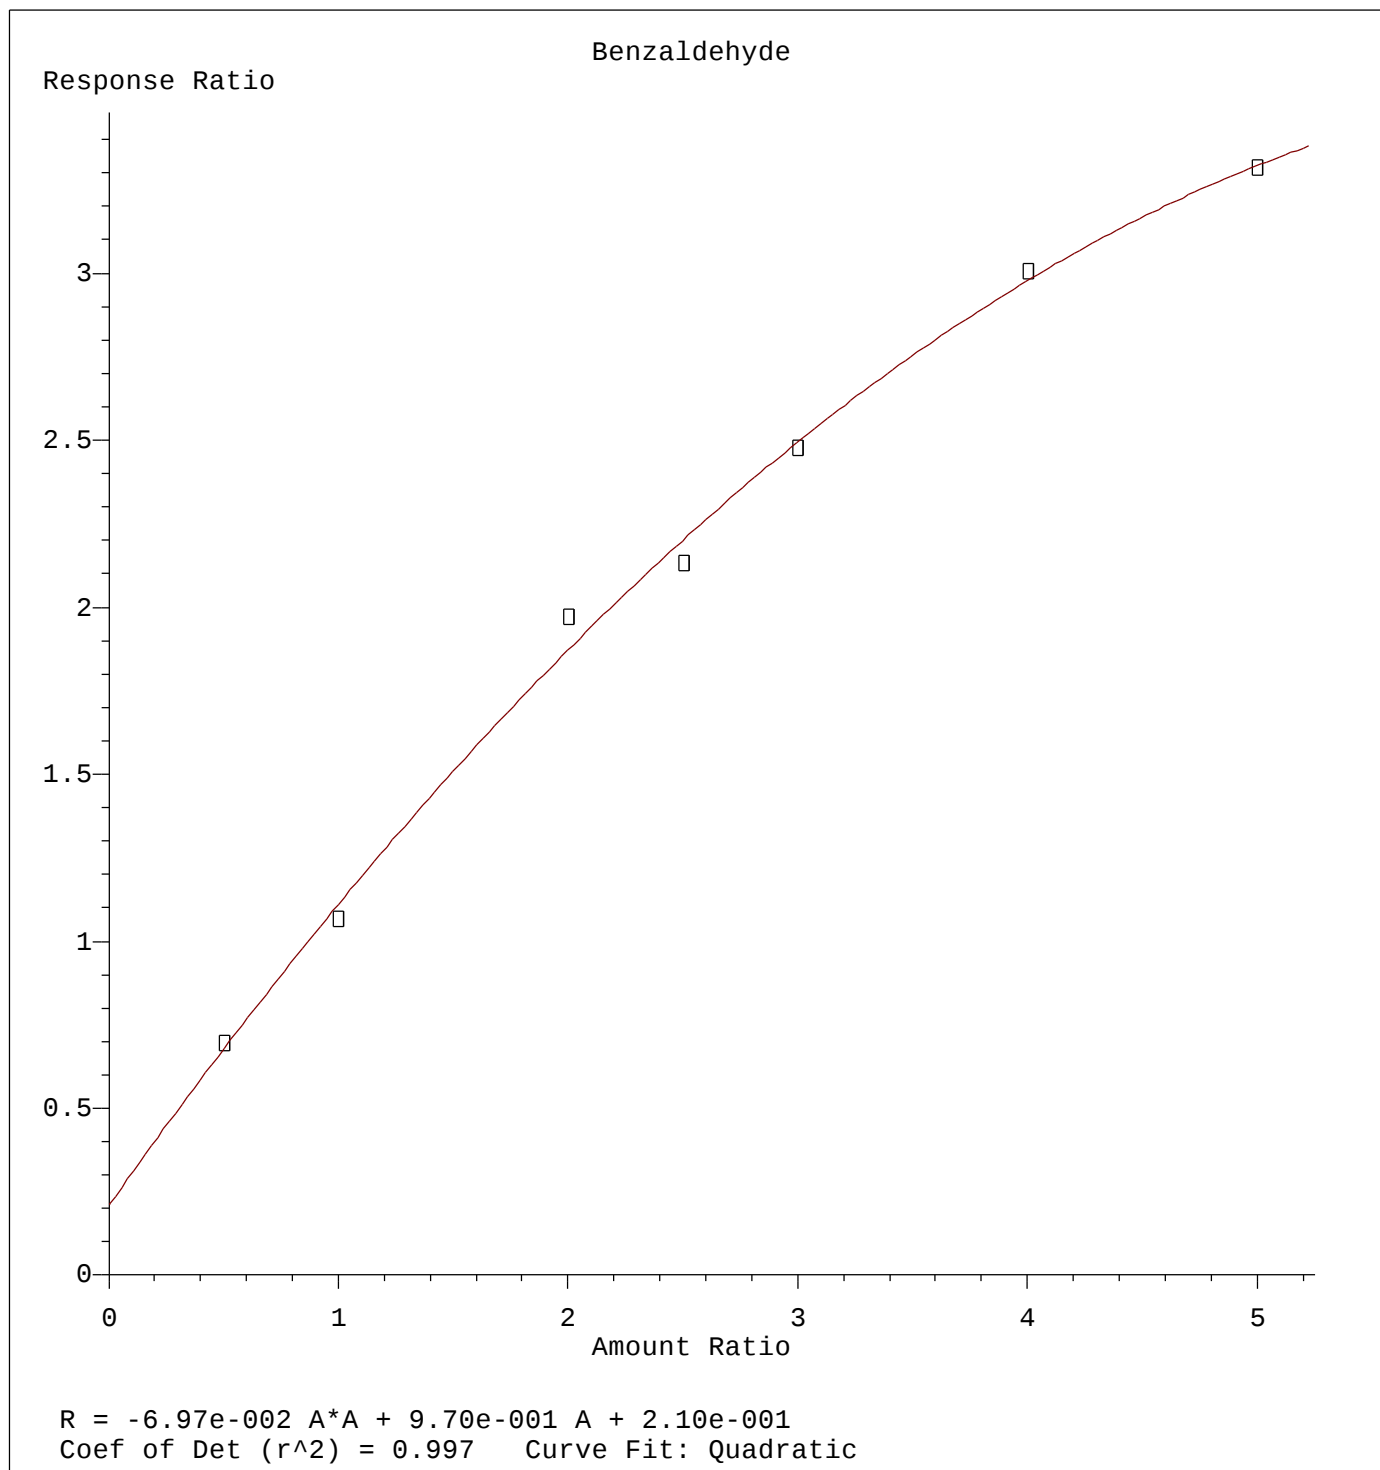

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
Calibration Table Last Updated: Wed Aug 28 13:34:15 2019

Indeno(1,2,3-cd)pyrene

Response Ratio

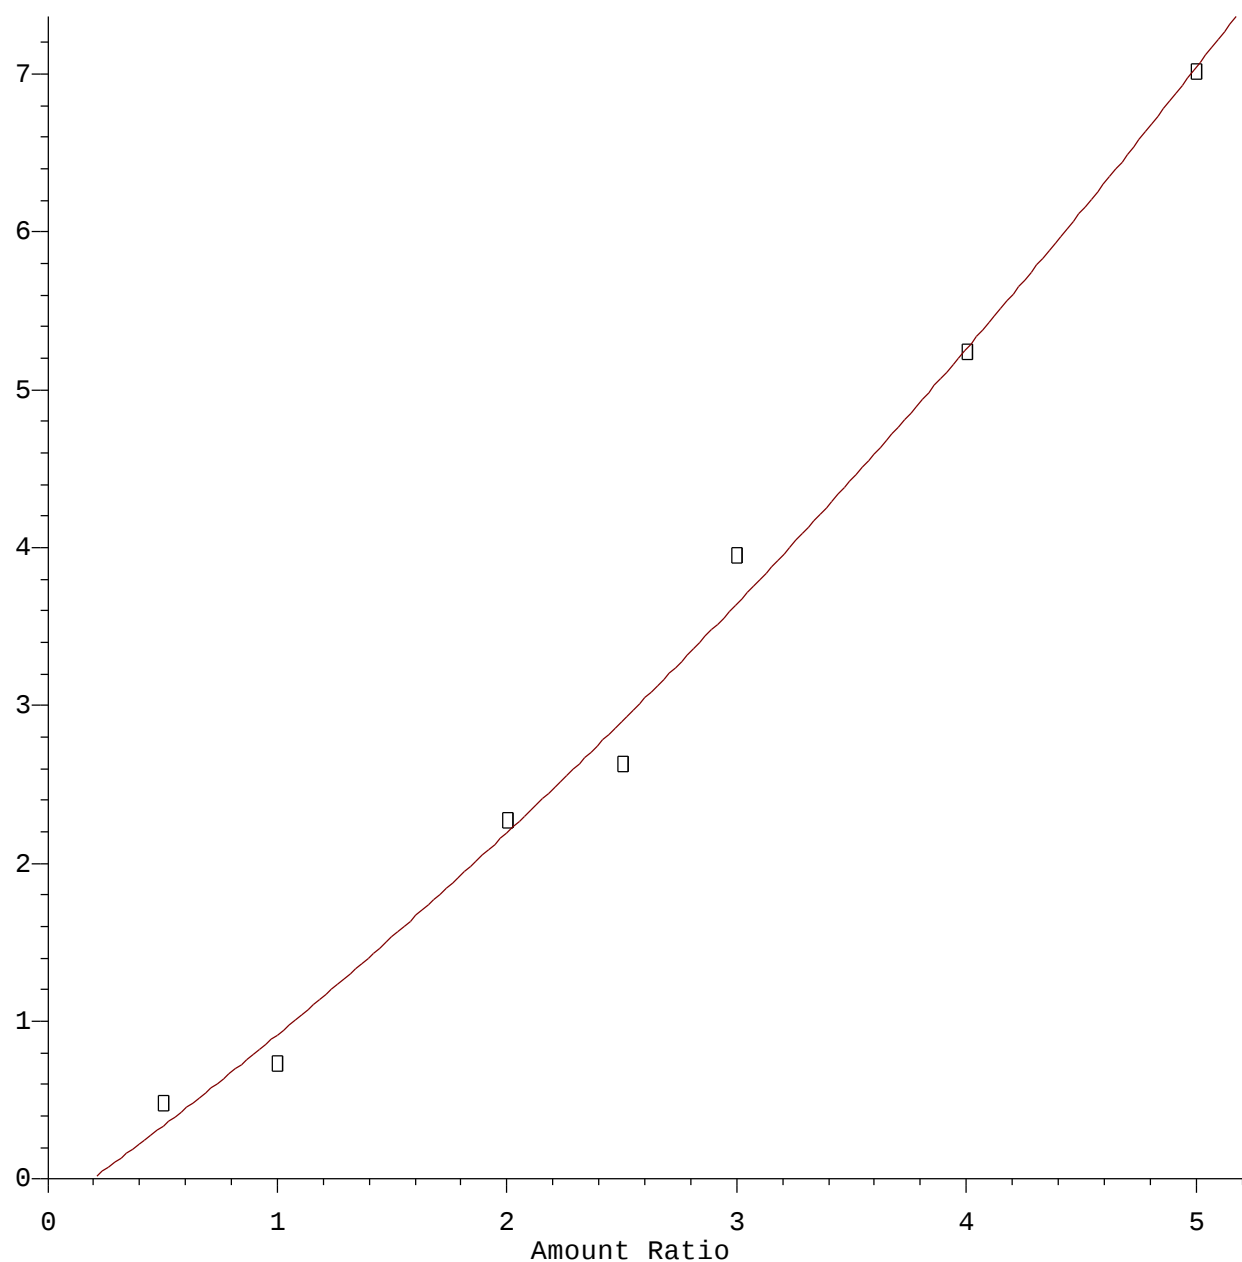

$R = 8.31e-002 A^2 + 1.03e+000 A - 2.01e-001$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
Calibration Table Last Updated: Wed Aug 28 13:34:15 2019