


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082819\
 Data File : BF116603.D
 Acq On : 28 Aug 2019 8:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 28 13:34:15 2019

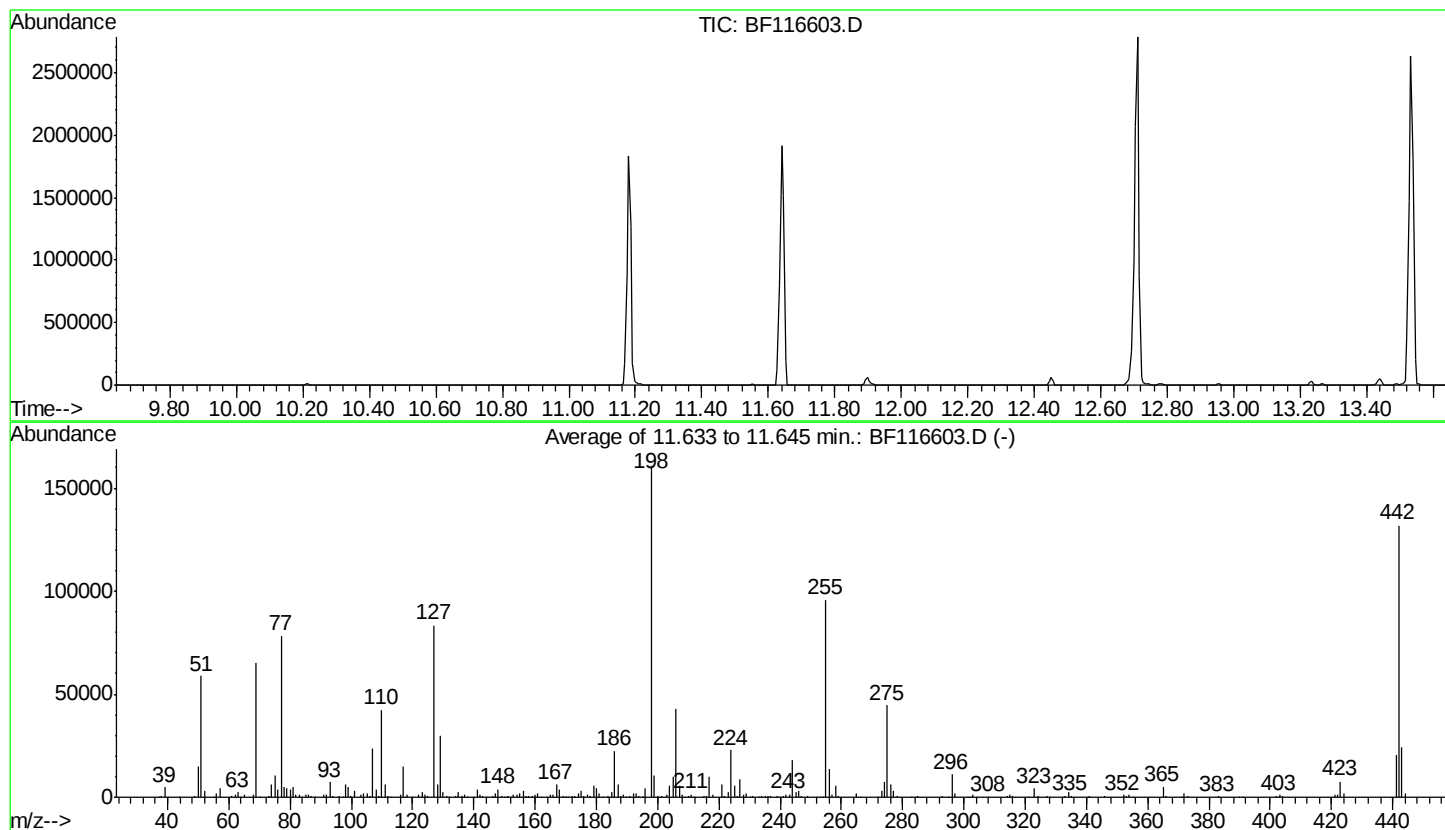

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	58928	PASS
68	69	0.00	2	1.8	1201	PASS
69	198	0.00	100	40.5	65157	PASS
70	69	0.00	2	0.2	141	PASS
127	198	10	80	51.9	83472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160912	PASS
199	198	5	9	6.6	10637	PASS
275	198	10	60	27.7	44592	PASS
365	198	1	100	3.2	5083	PASS
441	198	0.01	100	12.6	20216	PASS
442	198	50	100	81.9	131805	PASS
443	442	15	24	18.4	24251	PASS