


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082819\
 Data File : BF116619.D
 Acq On : 28 Aug 2019 17:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 28 13:34:15 2019

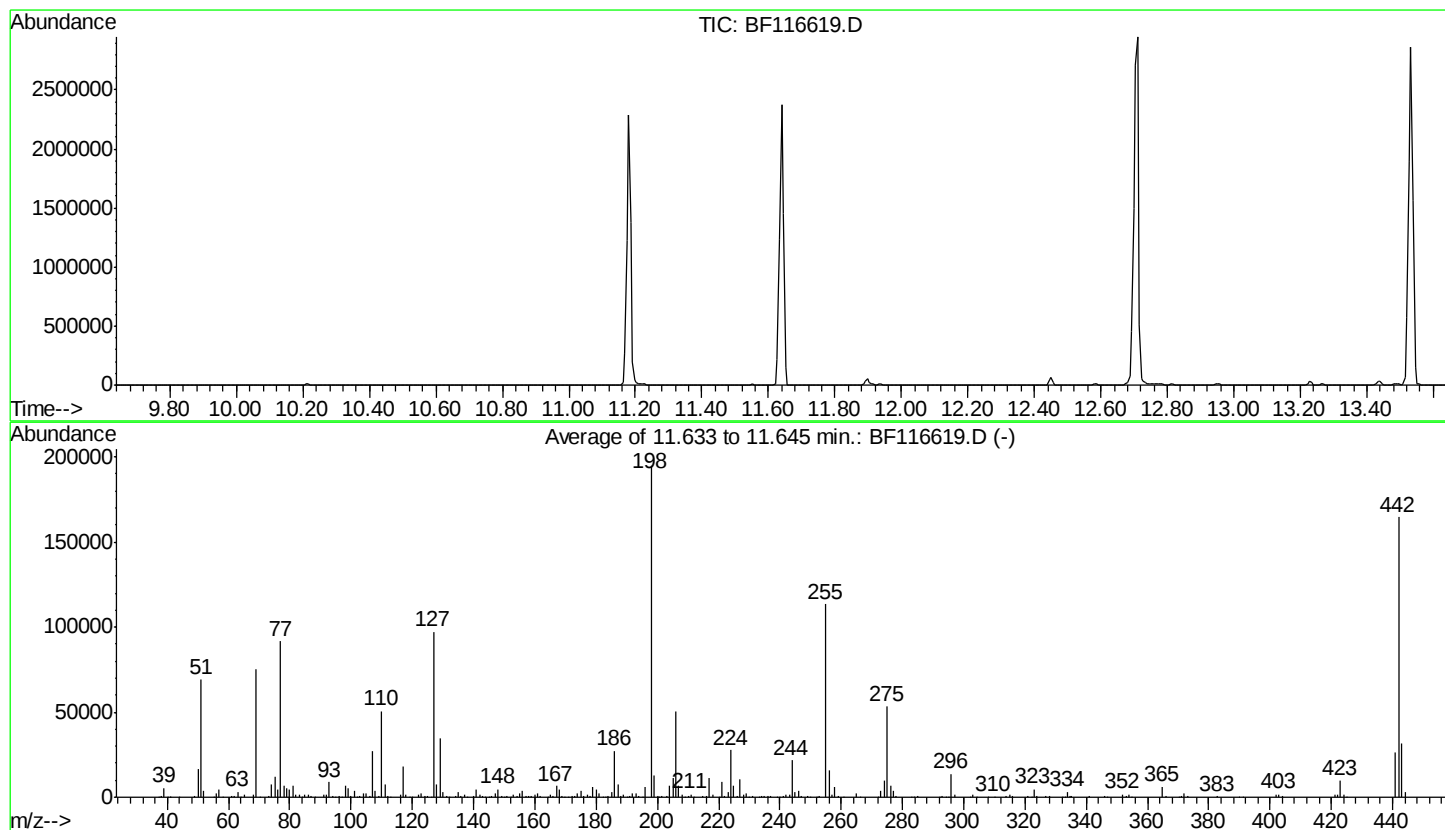

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	69178	PASS
68	69	0.00	2	1.8	1394	PASS
69	198	0.00	100	38.8	75573	PASS
70	69	0.00	2	0.3	190	PASS
127	198	10	80	50.0	97437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	194901	PASS
199	198	5	9	6.6	12832	PASS
275	198	10	60	27.3	53248	PASS
365	198	1	100	3.2	6200	PASS
441	198	0.01	100	13.5	26271	PASS
442	198	50	100	84.4	164528	PASS
443	442	15	24	19.4	31883	PASS