
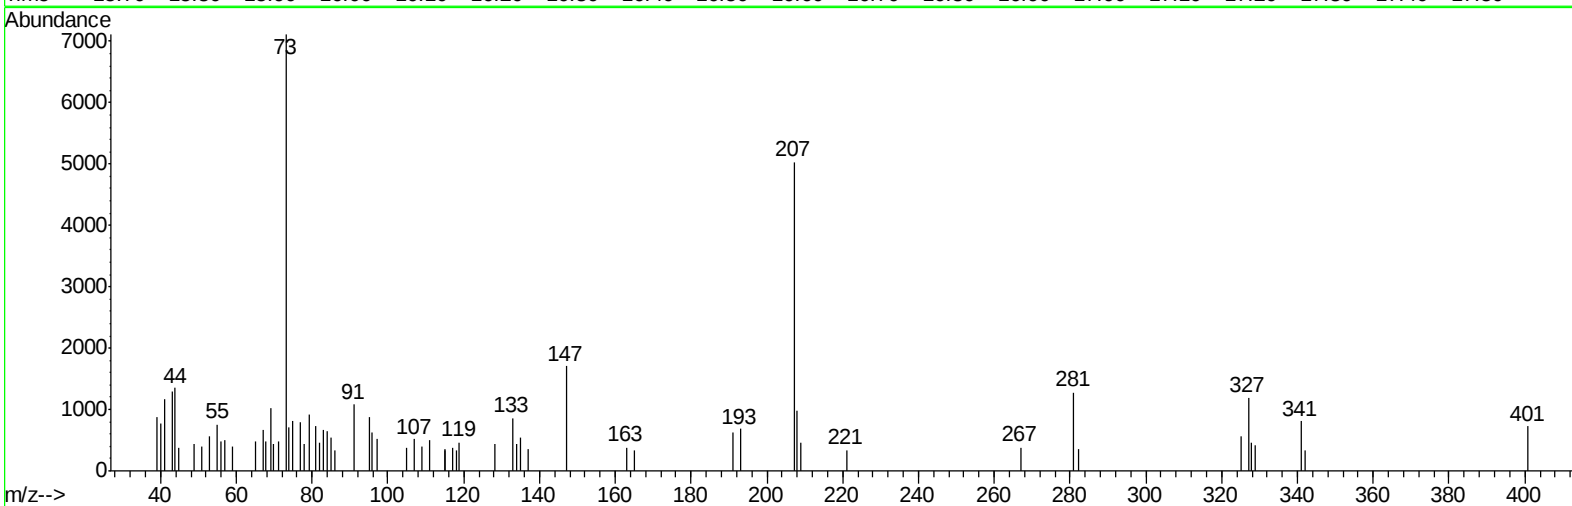


Data File : BN007526.D
Acq On : 01 Sep 2019 14:57
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 01:12:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

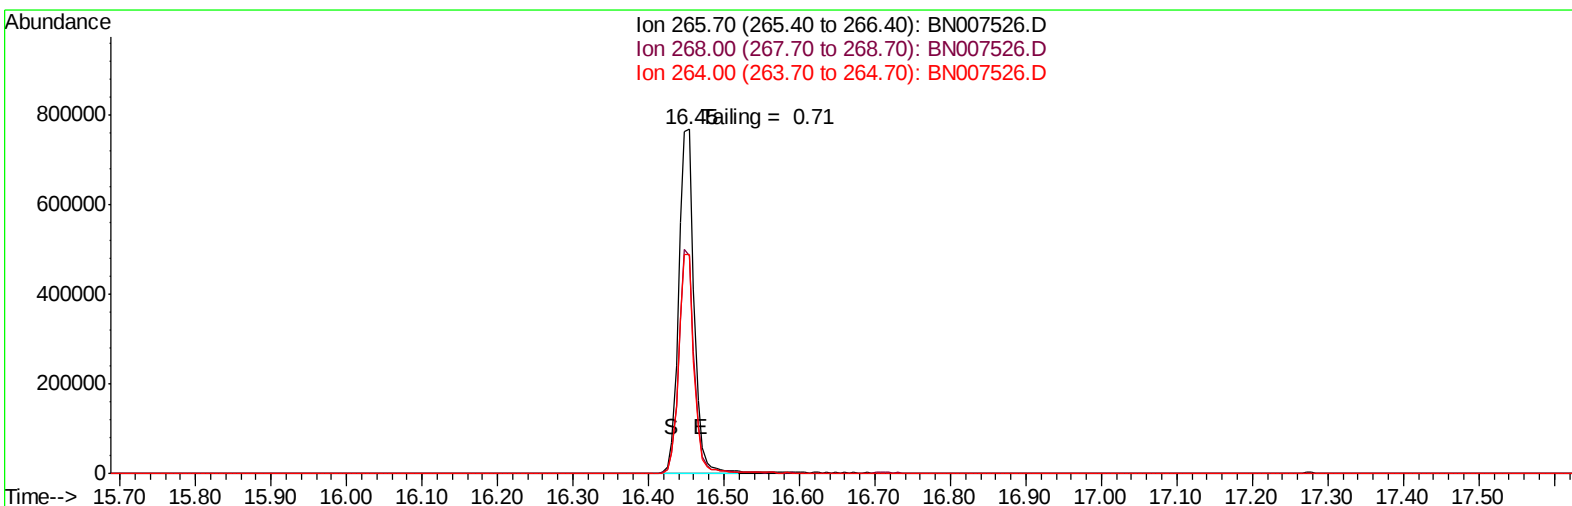

TIC: BN007526.D

(70) Pentachlorophenol (C)

11.169min (-11.169) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	64.00	0.00#
264.00	64.90	0.00#
0.00	0.00	0.00