
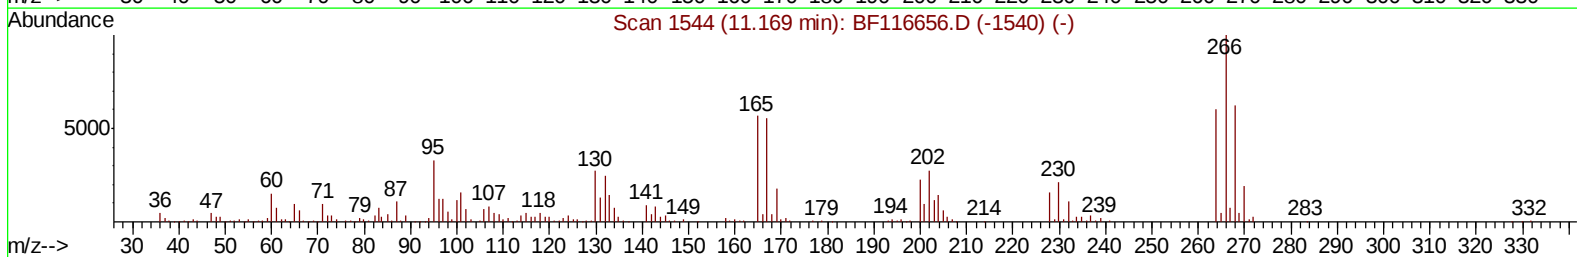
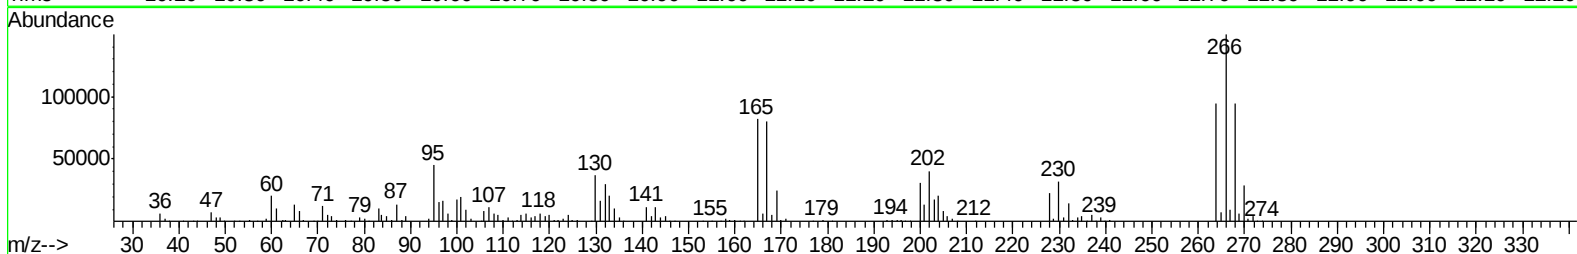


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083119\
Data File : BF116687.D
Acq On : 31 Aug 2019 9:15
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 01:37:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

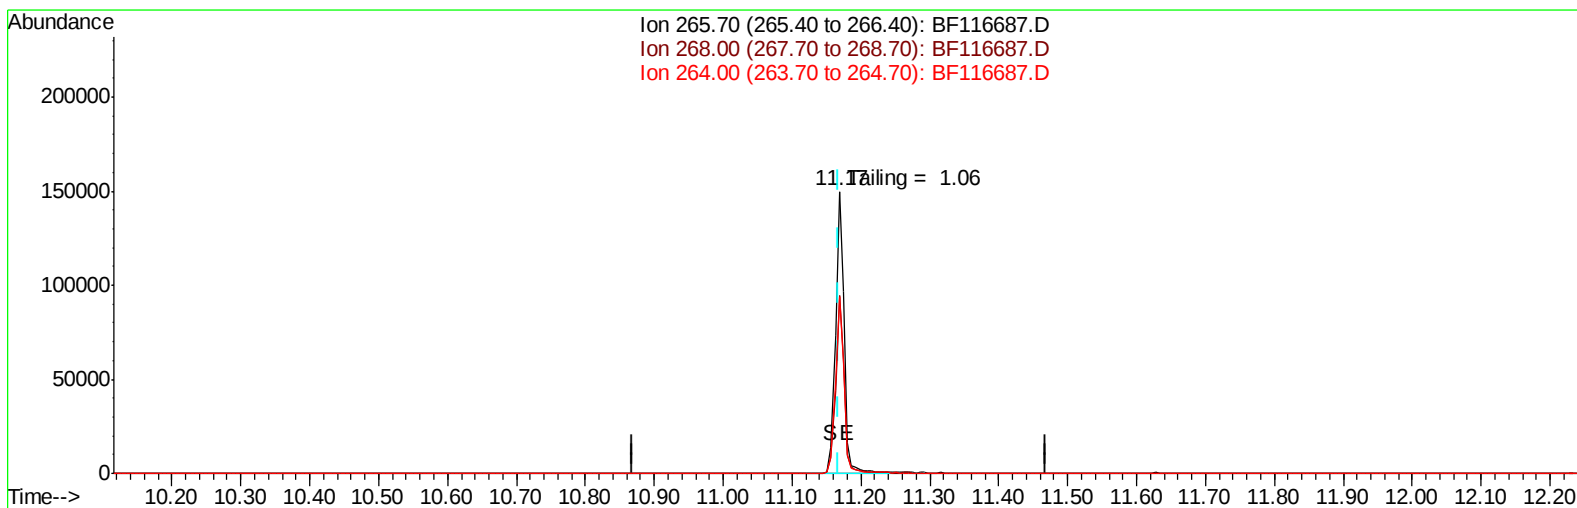

TIC: BF116687.D

(70) Pentachlorophenol (C)




11.169min (+0.000) 72402.57ng

response 129547

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.17
264.00	64.90	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083119\
Data File : BF116687.D
Acq On : 31 Aug 2019 9:15
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 01:37:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

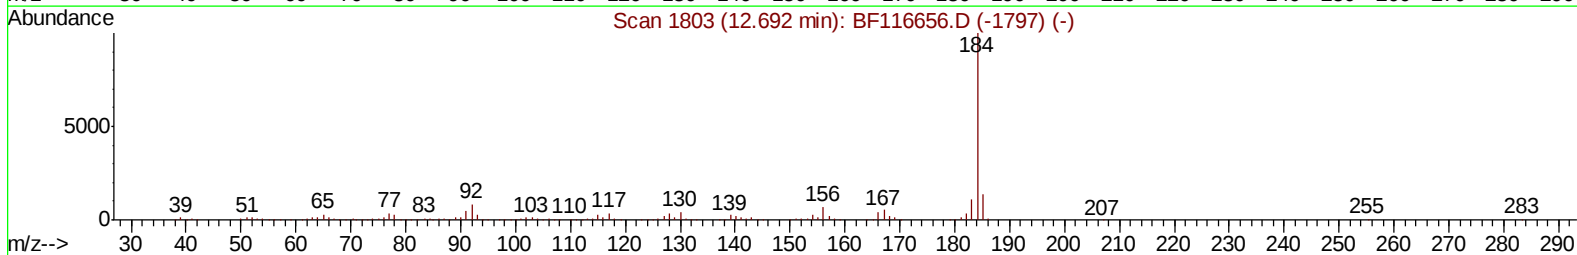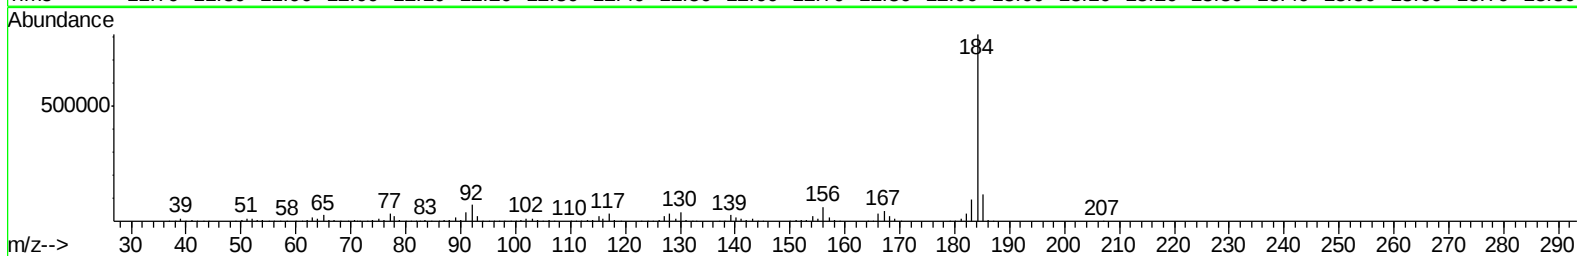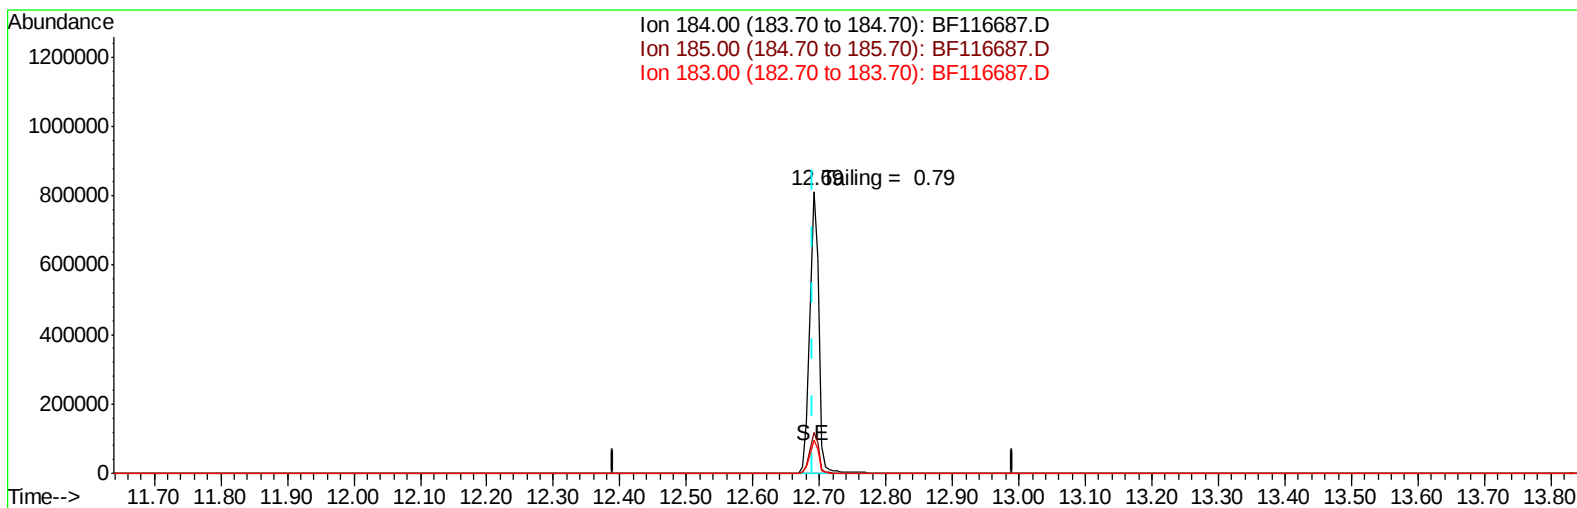

TIC: BF116687.D

(77) Benzidine

12.692min (+0.001) 164856.84ng

response 788863

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.49
183.00	11.50	11.63
0.00	0.00	0.00