
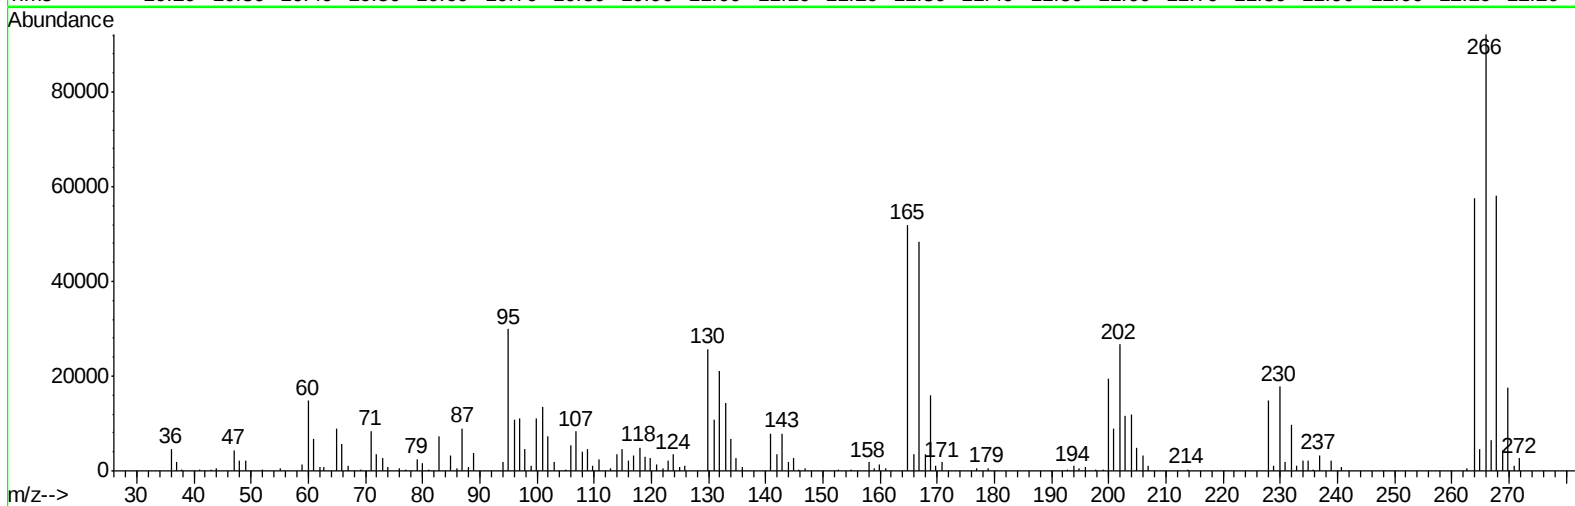


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
Data File : BF116711.D
Acq On : 31 Aug 2019 22:28
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:52:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

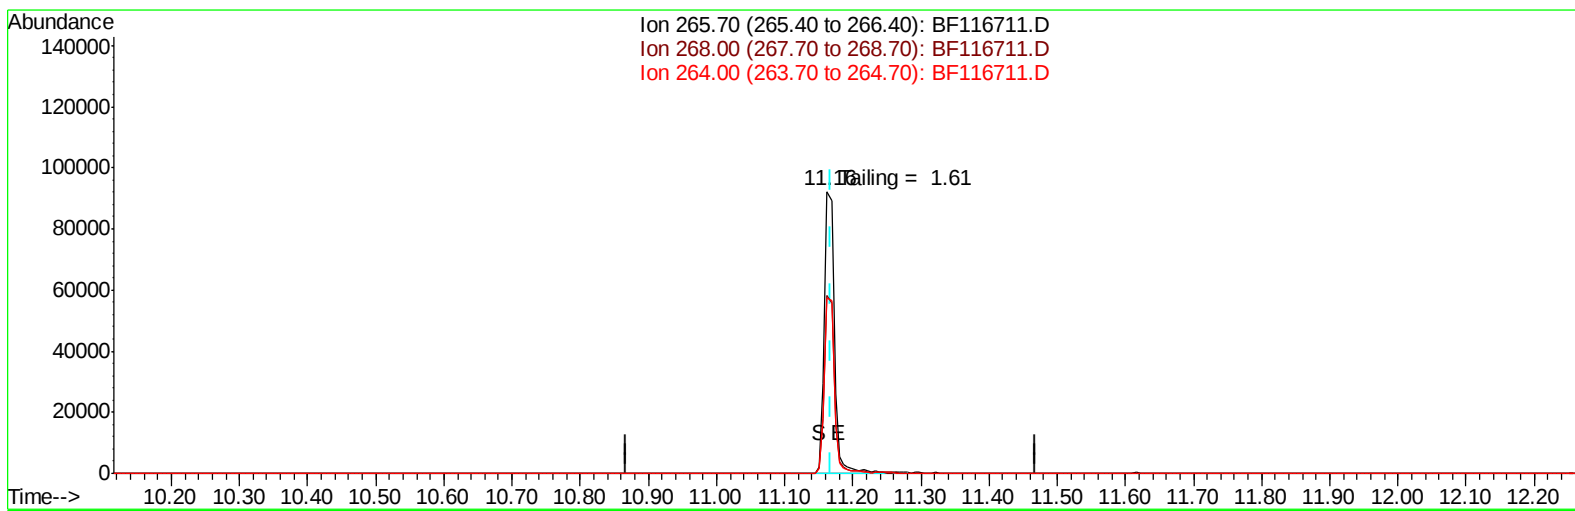

TIC: BF116711.D

(70) Pentachlorophenol (C)



11.163min (-0.006) 154933.80ng

response 91609

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.11
264.00	64.90	62.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
Data File : BF116711.D
Acq On : 31 Aug 2019 22:28
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 06:52:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

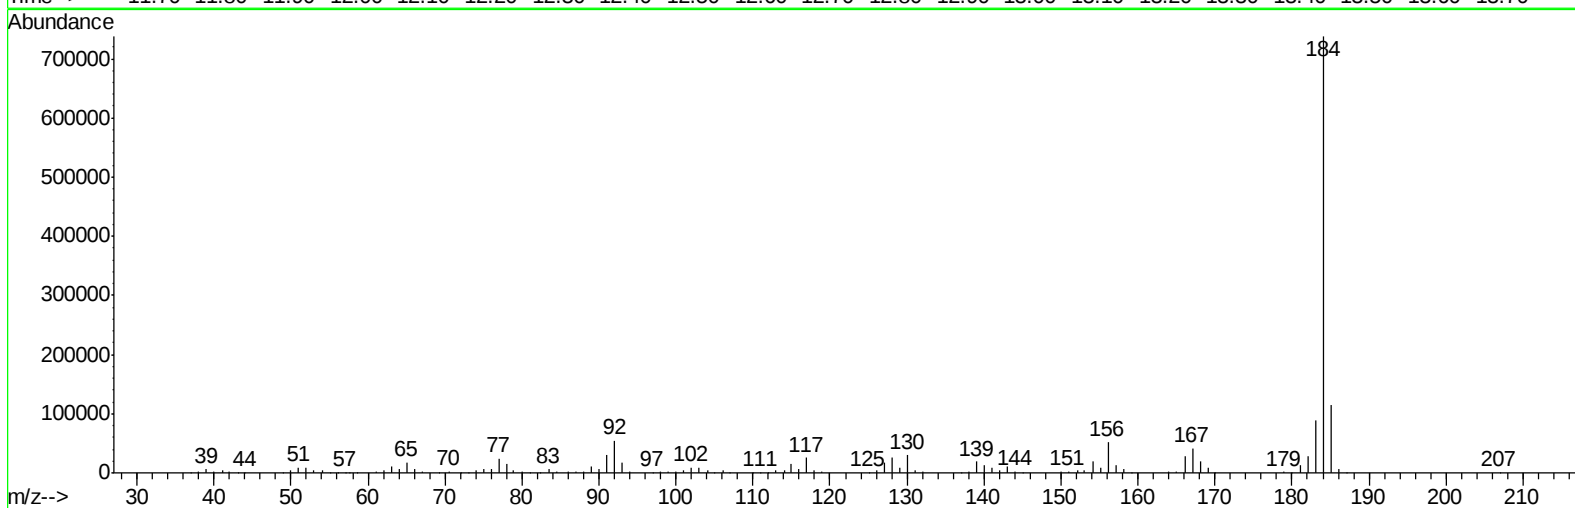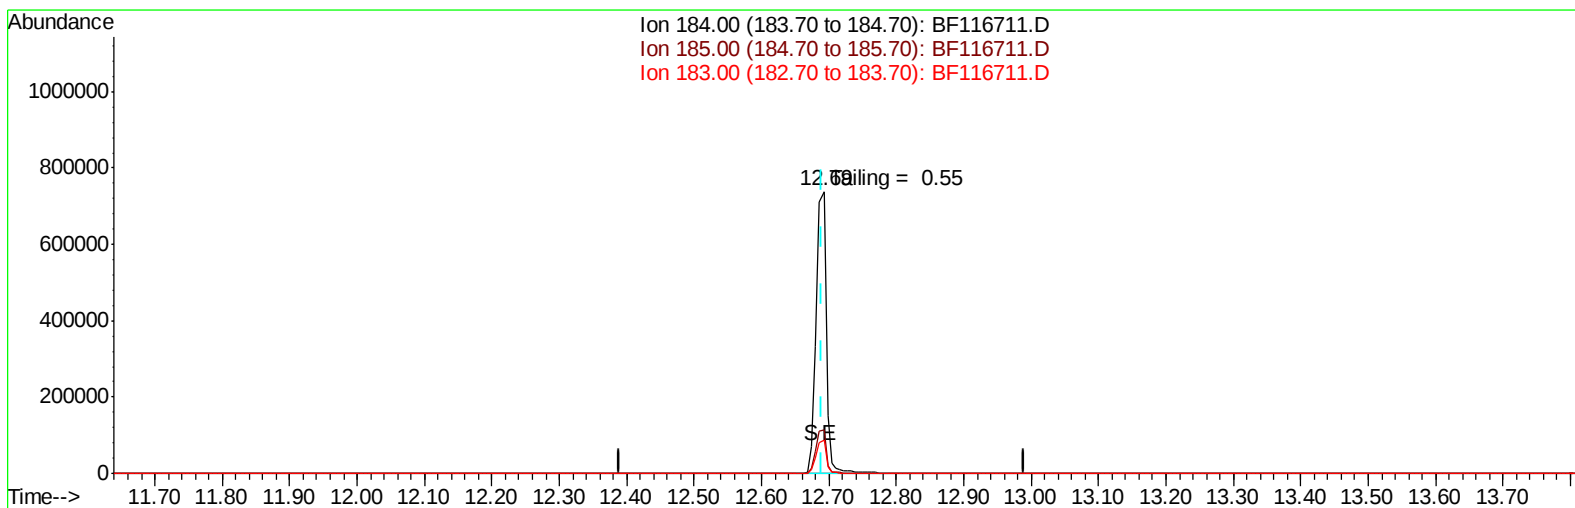

TIC: BF116711.D

(77) Benzidine

12.692min (+0.001) 0.00ng

response 743191

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.41
183.00	11.50	11.91
0.00	0.00	0.00