

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
 Data File : BF116706.D
 Acq On : 31 Aug 2019 18:22
 Operator : HP/JU
 Sample : K4619-36
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP12-COMP

Quant Time: Sep 01 01:11:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 30 20:02:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	109493	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	424637	20.00	ng	0.00
39) Acenaphthene-d10	9.88	164	221583	20.00	ng	0.00
64) Phenanthrene-d10	11.36	188	355131	20.00	ng	0.00
76) Chrysene-d12	13.99	240	219839	20.00	ng	0.00
87) Perylene-d12	15.44	264	242954	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	734503	108.68	ng	0.00
7) Phenol-d6	6.47	99	1017348	114.63	ng	0.00
23) Nitrobenzene-d5	7.40	82	632979	85.10	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	187275	126.42	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	1068972	81.38	ng	0.00
79) Terphenyl-d14	12.95	244	946816	79.67	ng	0.00
Target Compounds						
10) Phenol	6.49	94	25511	2.596	ng	92
50) Dimethylphthalate	9.59	163	150987	9.870	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
Data File : BF116706.D
Acq On : 31 Aug 2019 18:22
Operator : HP/JU
Sample : K4619-36
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP12-COMP

Quant Time: Sep 01 01:11:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

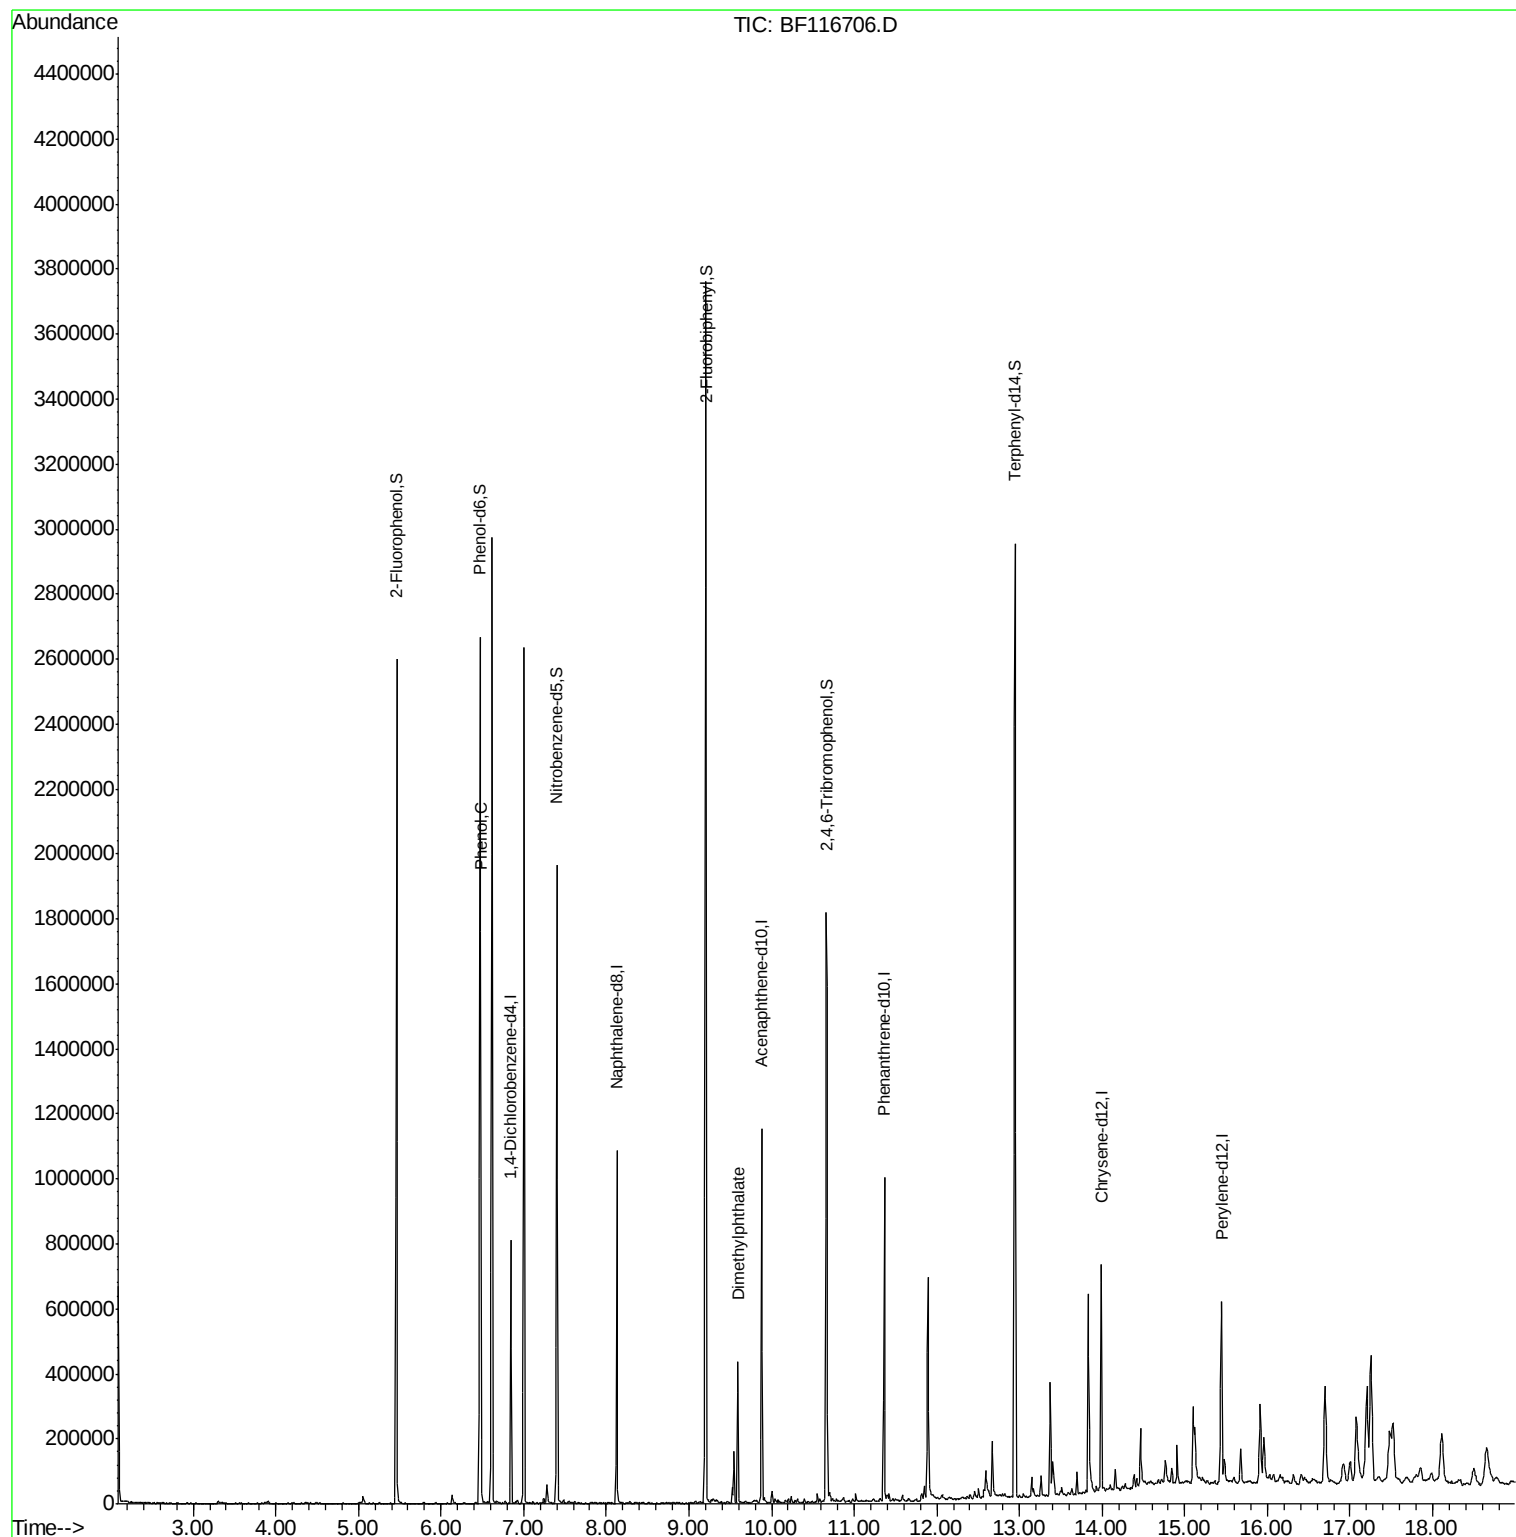



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.85 min Scan# 809

Delta R.T. -0.01 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22

Instrument :

BNA_F

ClientSampleId :

TP12-COMP


Tot Ion:152 Resp: 109493

Ion Ratio Lower Upper

152 100

150 153.5 124.4 186.6

115 63.5 49.9 74.9



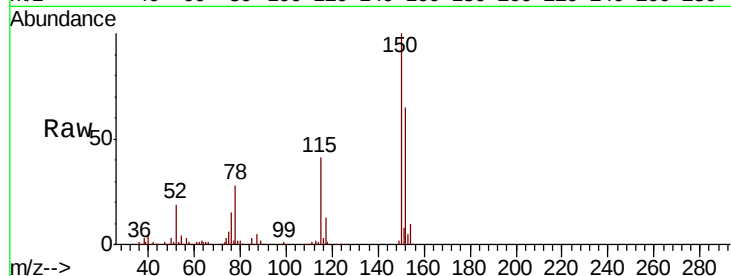


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

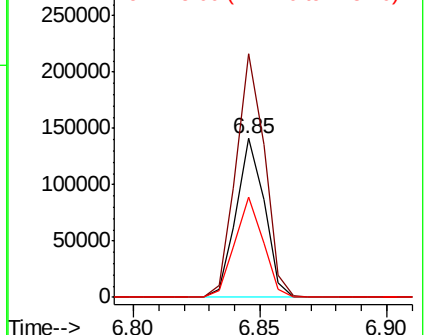

#5

2-Fluorophenol

Concen: 108.677 ng

RT: 5.46 min Scan# 574

Delta R.T. 0.00 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22


Tgt Ion:112 Resp: 734503

Ion Ratio Lower Upper

112 100

64 57.5 47.1 70.7

63 29.7 24.9 37.3





Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

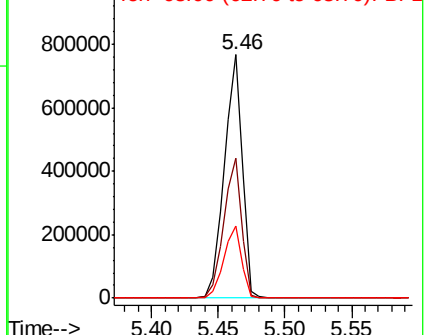



#7

Phenol-d6

Concen: 114.634 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.01 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22

Instrument :

BNA_F

ClientSampleId :

TP12-COMP


Tot Ion: 99 Resp: 1017348

Ion Ratio Lower Upper




99 100

42 16.2 13.7 20.5

71 36.1 30.8 46.2

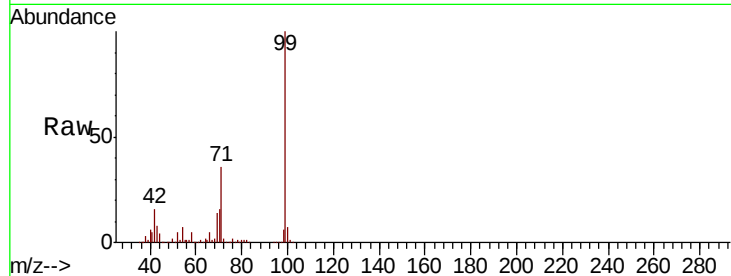

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

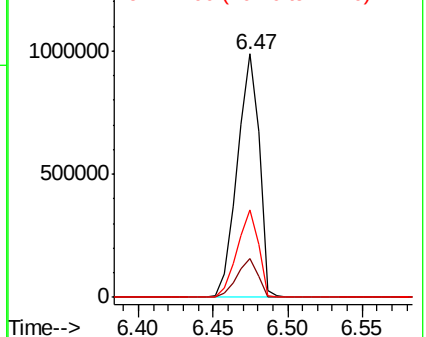

#10

Phenol

Concen: 2.596 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22


Tgt Ion: 94 Resp: 25511

Ion Ratio Lower Upper



94 100

65 25.9 10.8 50.8

66 36.6 21.1 61.1



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



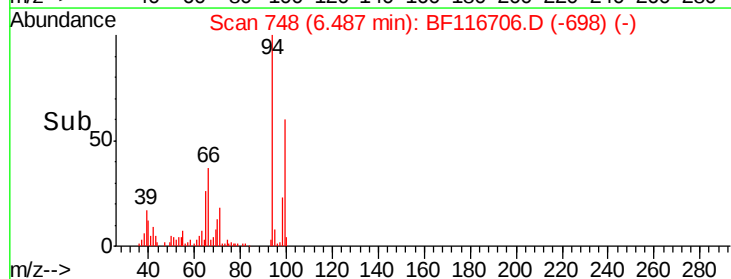
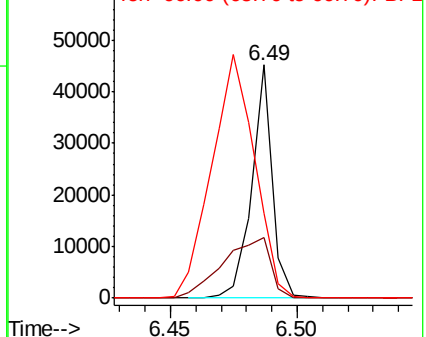




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1027
Delta R.T. -0.01 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22




Instrument :
BNA_F
ClientSampleId :
TP12-COMP

Tot Ion:136	Resp:	424637
Ion Ratio	Lower	Upper
136 100		
137 11.3	8.9	13.3
54 6.1	4.8	7.2
68 5.2	4.0	6.0

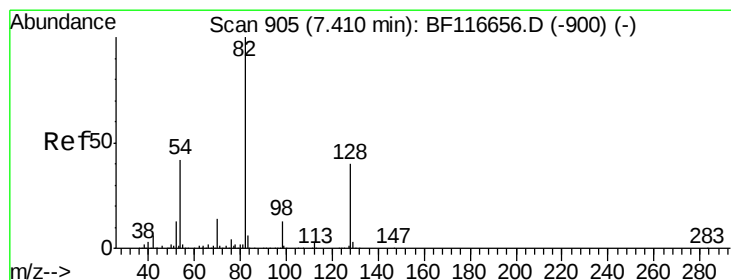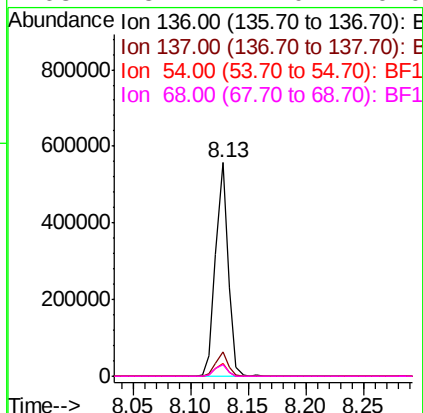

#23
Nitrobenzene-d5
Concen: 85.096 ng
RT: 7.40 min Scan# 904
Delta R.T. -0.01 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22

Tgt Ion: 82	Resp: 632979
Ion Ratio	Lower Upper
82 100	
128 41.0	32.8 49.2
54 41.5	36.9 55.3

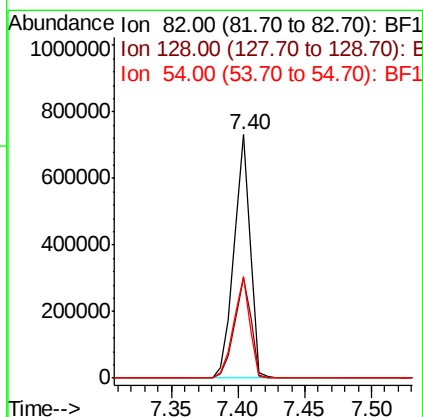







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.88 min Scan# 1325
Delta R.T. -0.01 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22

Instrument :
BNA_F
ClientSampleId :
TP12-COMP

Tot Ion:164 Resp: 221583
Ion Ratio Lower Upper
164 100
162 100.1 81.4 122.0
160 43.4 35.4 53.2

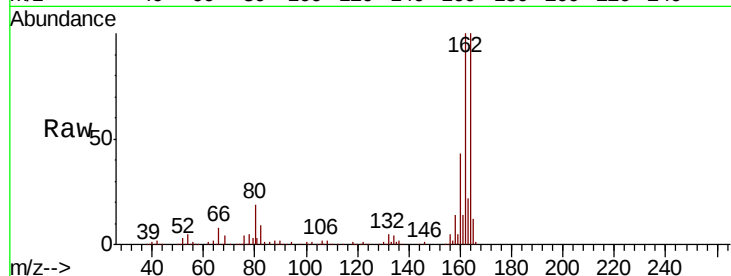


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


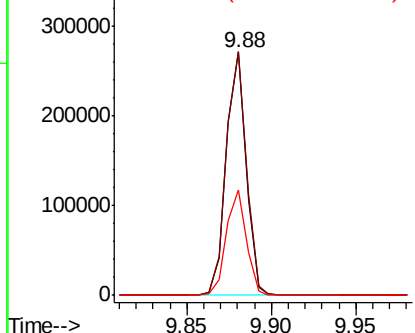


#42
2,4,6-Tribromophenol
Concen: 126.424 ng
RT: 10.67 min Scan# 1459
Delta R.T. -0.01 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22

Tgt Ion:330 Resp: 187275
Ion Ratio Lower Upper
330 100
332 97.0 76.9 115.3
141 45.2 31.4 47.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




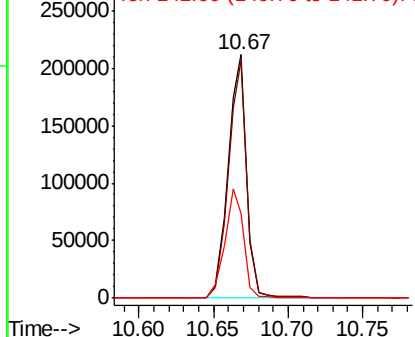




#45
2-Fluorobiphenyl
Concen: 81.380 ng
RT: 9.20 min Scan# 1210
Delta R.T. -0.00 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22




Instrument :
BNA_F
ClientSampleId :
TP12-COMP


Tot Ion:172 Resp: 1068972
Ion Ratio Lower Upper
172 100
171 35.8 27.8 41.6
170 24.1 18.9 28.3

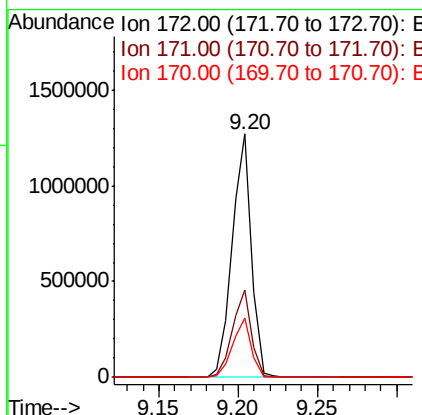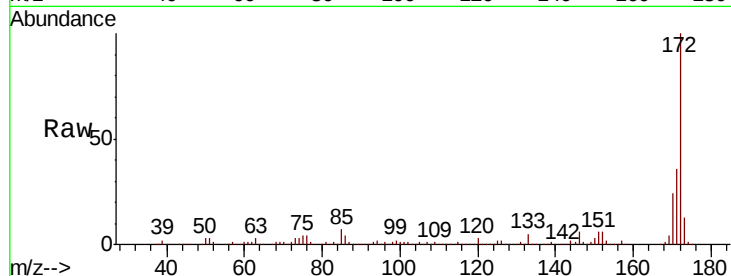

#50
Dimethylphthalate
Concen: 9.870 ng
RT: 9.59 min Scan# 1276
Delta R.T. -0.02 min
Lab File: BF116706.D
Acq: 31 Aug 2019 18:22

Tgt Ion:163 Resp: 150987
Ion Ratio Lower Upper
163 100
194 3.8 2.8 4.2
164 9.8 8.6 12.8

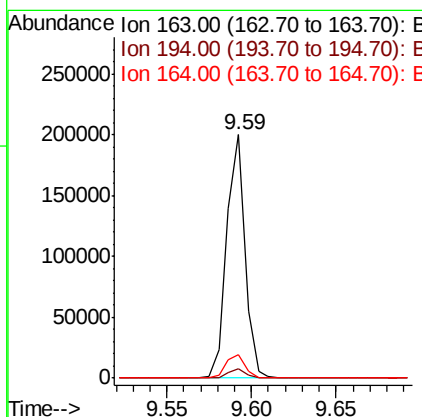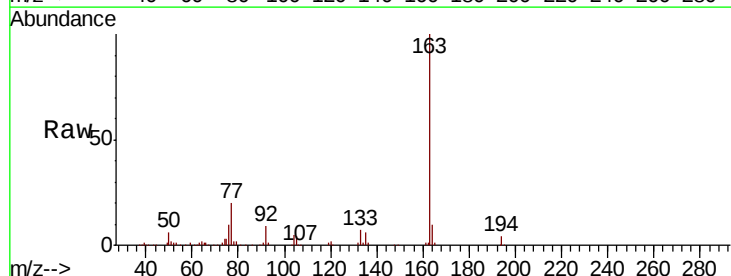



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1577

Delta R.T. -0.01 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22

Instrument :

BNA_F

ClientSampleId :

TP12-COMP


Tot Ion:188 Resp: 355131

Ion Ratio Lower Upper

188 100

94 9.3 7.3 10.9




80 10.8 8.4 12.6



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

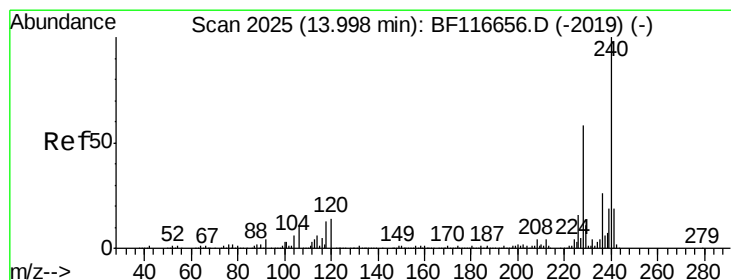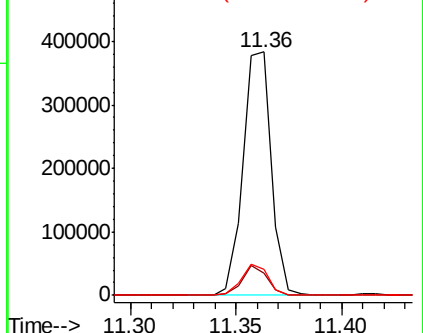

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.01 min

Lab File: BF116706.D

Acq: 31 Aug 2019 18:22


Tgt Ion:240 Resp: 219839

Ion Ratio Lower Upper

240 100

120 12.6 9.1 13.7



236 25.8 21.1 31.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




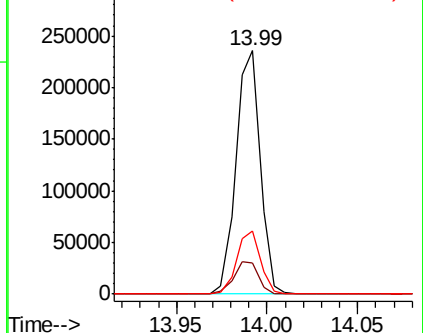


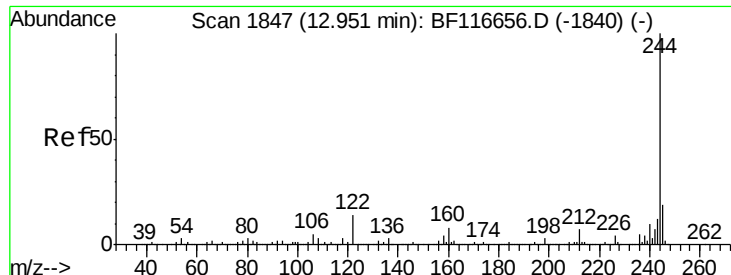

#79
 Terphenyl-d14
 Concen: 79.674 ng
 RT: 12.95 min Scan# 1846
 Delta R.T. -0.01 min
 Lab File: BF116706.D
 Acq: 31 Aug 2019 18:22

Instrument :
 BNA_F
 ClientSampleId :
 TP12-COMP

Tot Ion:244 Resp: 946816
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.1 9.1
 122 14.1 10.2 15.4

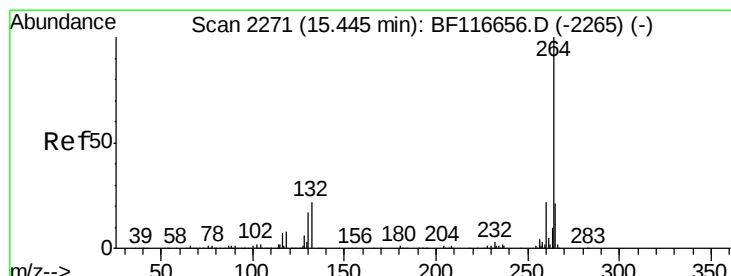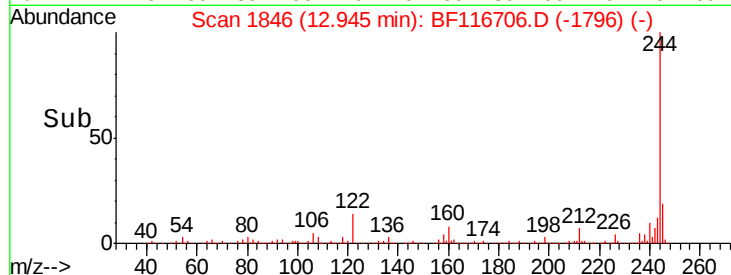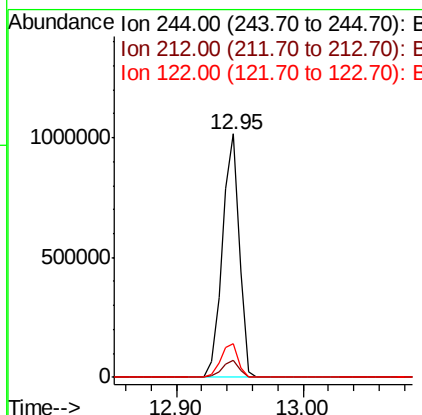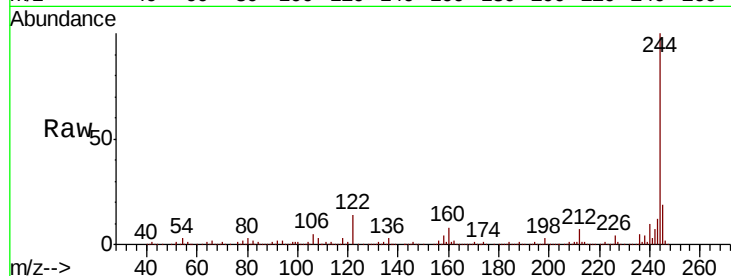

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2271
 Delta R.T. 0.00 min
 Lab File: BF116706.D
 Acq: 31 Aug 2019 18:22

Tgt Ion:264 Resp: 242954
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.3 27.5
 265 21.4 16.5 24.7

