

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
 Data File : BF116715.D
 Acq On : 1 Sep 2019 00:27
 Operator : HP/JU
 Sample : K4527-37
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T9-12-13-P-(0-1.9)

Quant Time: Sep 01 01:33:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 30 20:02:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	113734	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	446764	20.00	ng	0.00
39) Acenaphthene-d10	9.88	164	226950	20.00	ng	0.00
64) Phenanthrene-d10	11.36	188	375840	20.00	ng	-0.01
76) Chrysene-d12	13.99	240	248746	20.00	ng	-0.01
87) Perylene-d12	15.44	264	276236	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	831486	118.44	ng	0.00
7) Phenol-d6	6.47	99	1045851	113.45	ng	0.00
23) Nitrobenzene-d5	7.40	82	760226	97.14	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	238005	156.87	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	1268008	94.25	ng	0.00
79) Terphenyl-d14	12.94	244	1260685	93.76	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083119\
Data File : BF116715.D
Acq On : 1 Sep 2019 00:27
Operator : HP/JU
Sample : K4527-37
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T9-12-13-P-(0-1.9)

Quant Time: Sep 01 01:33:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

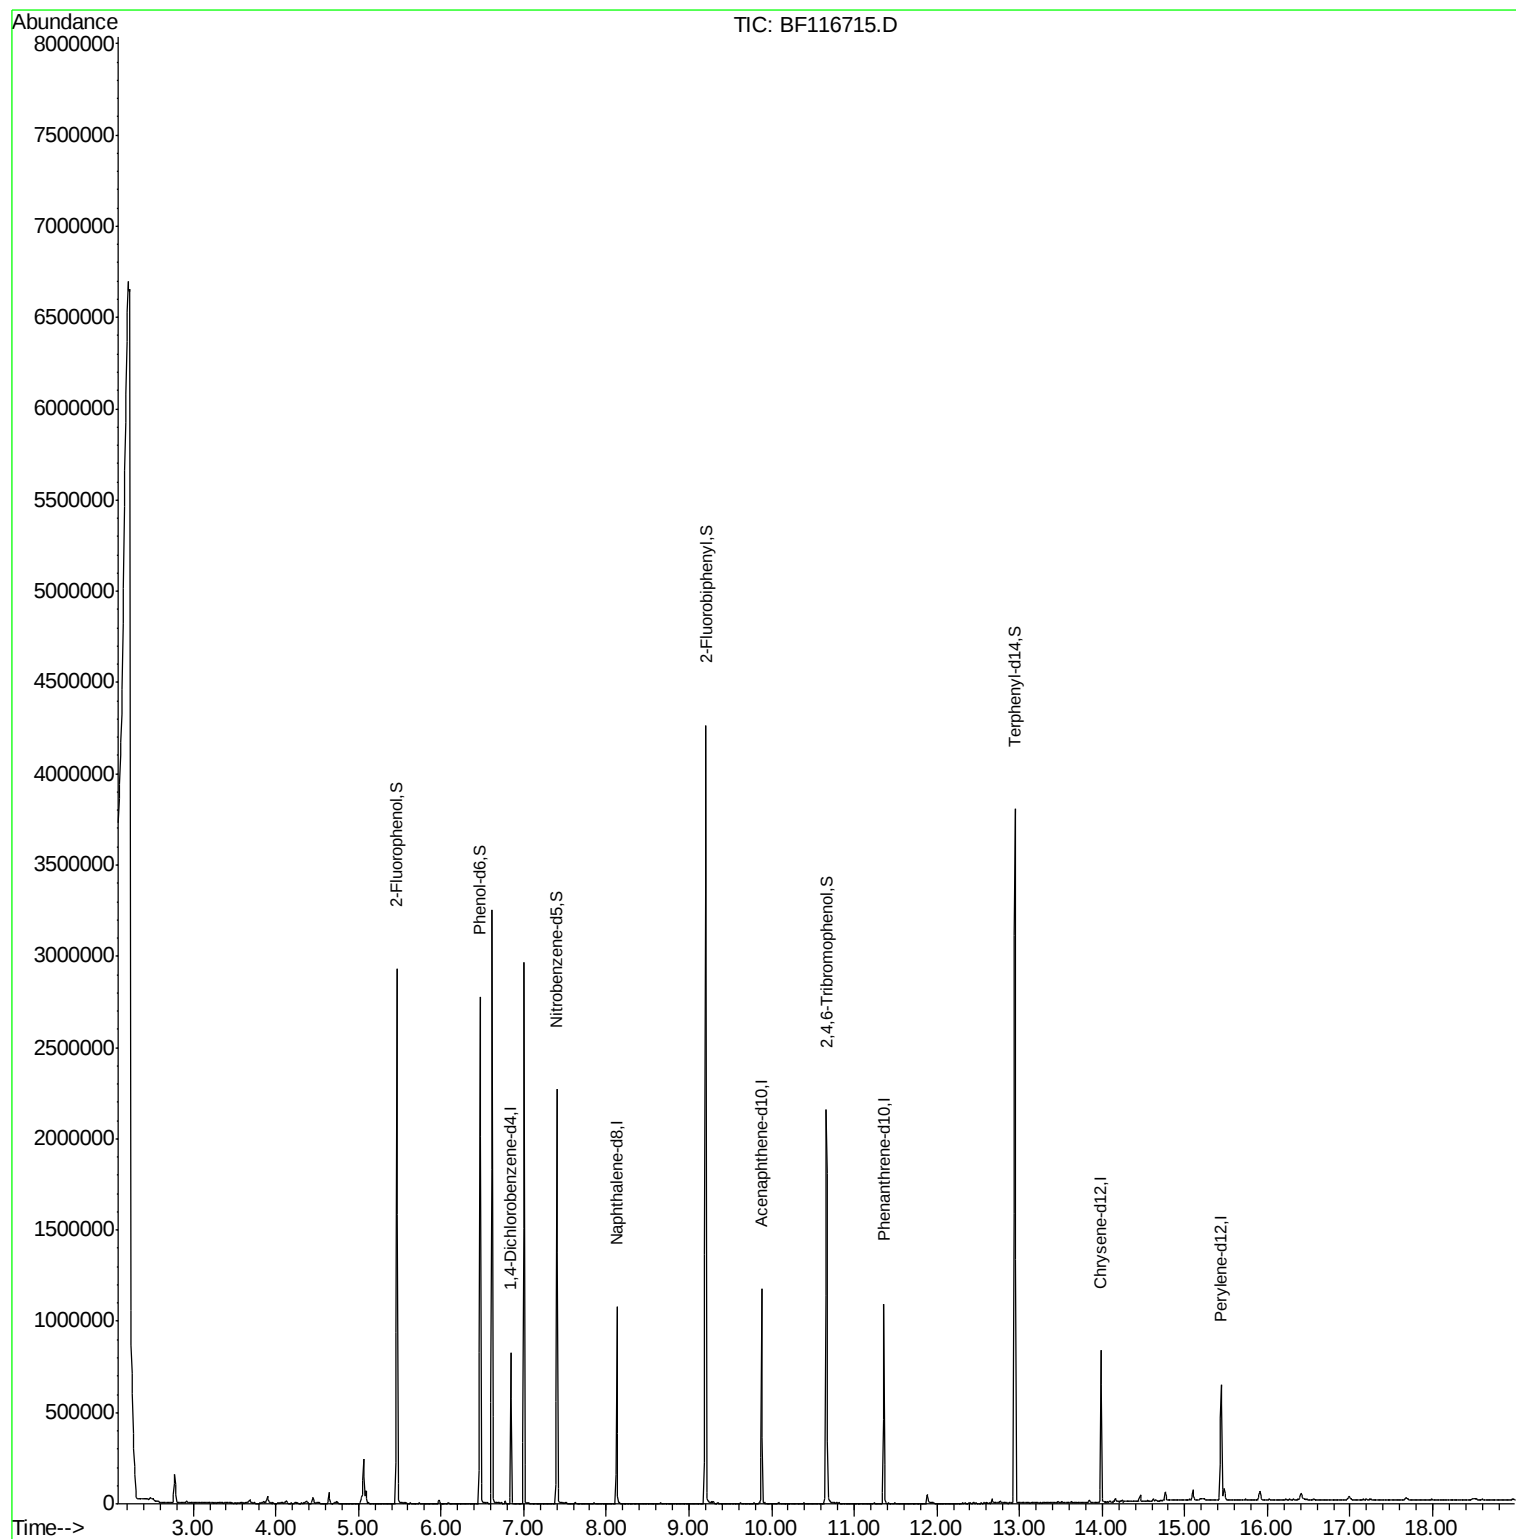




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 809
Delta R.T. -0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27

Instrument :
BNA_F
ClientSampleId :
T9-12-13-P-(0-1.9)

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.3	124.4	186.6
115	64.8	49.9	74.9


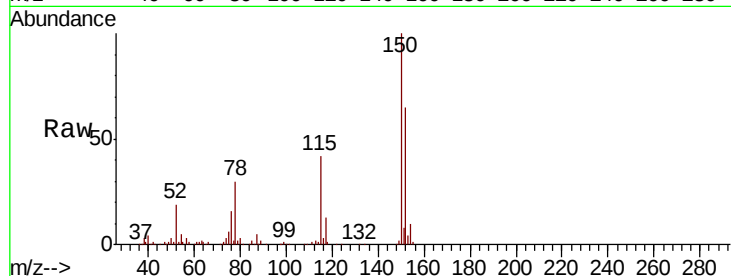


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

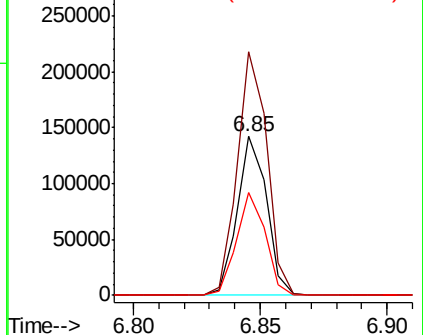

#5

2-Fluorophenol
Concen: 118.439 ng
RT: 5.47 min Scan# 575
Delta R.T. 0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.0	47.1	70.7
63	30.4	24.9	37.3


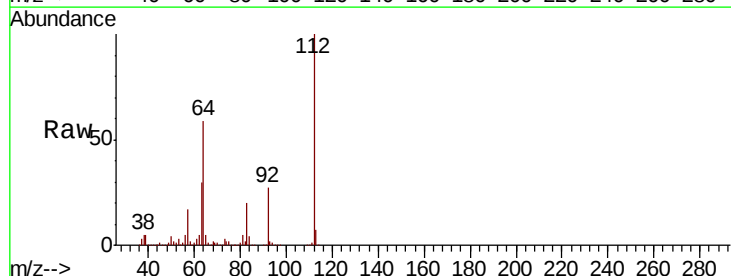


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

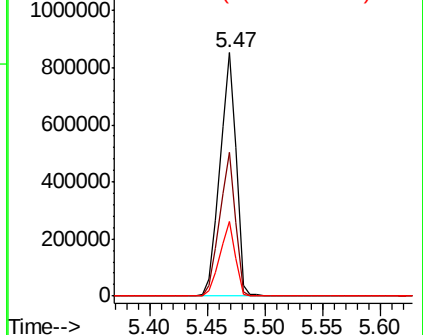



#7

Phenol-d6

Concen: 113.451 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.01 min

Lab File: BF116715.D

Acq: 1 Sep 2019 00:27

Instrument :


BNA_F

ClientSampleId :

T9-12-13-P-(0-1.9)

Tot Ion: 99 Resp: 1045851

Ion	Ratio	Lower	Upper
99	100		
42	15.8	13.7	20.5
71	35.1	30.8	46.2





Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.13 min Scan# 1027


Delta R.T. -0.01 min

Lab File: BF116715.D

Acq: 1 Sep 2019 00:27

Tgt Ion: 136 Resp: 446764

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	5.7	4.8	7.2
68	5.2	4.0	6.0




Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1








#23
Nitrobenzene-d5
Concen: 97.141 ng
RT: 7.40 min Scan# 904
Delta R.T. -0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27




Instrument :
BNA_F
ClientSampleId :
T9-12-13-P-(0-1.9)


Tot Ion	82	Resp	760226
Ion Ratio	100	Lower	Upper
128	41.7	32.8	49.2
54	42.4	36.9	55.3

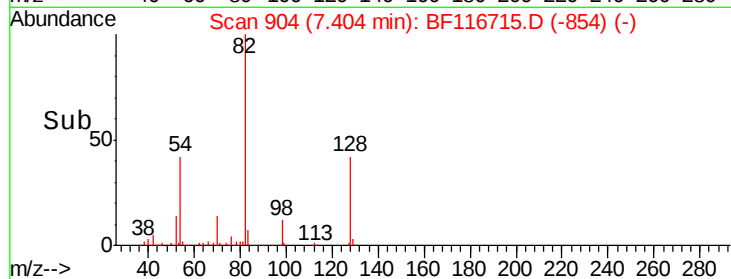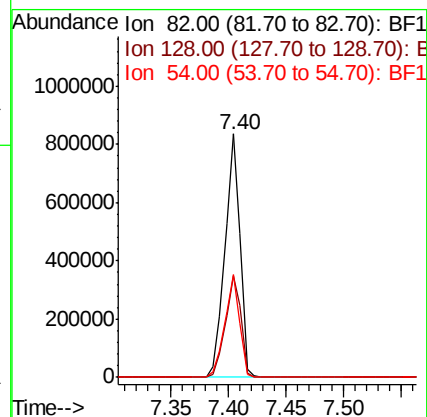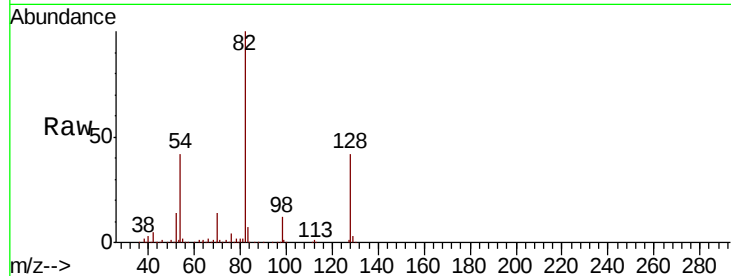

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.88 min Scan# 1325
Delta R.T. -0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27

Tgt Ion	164	Resp	226950
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	102.4	81.4	122.0
160	46.3	35.4	53.2

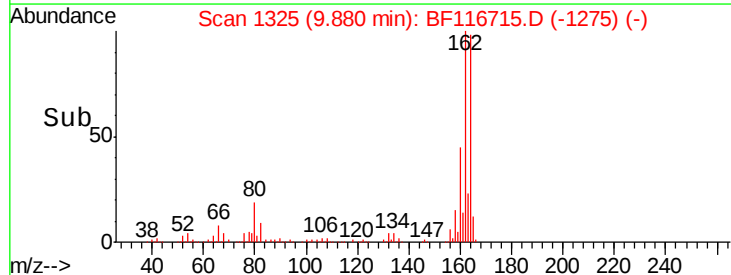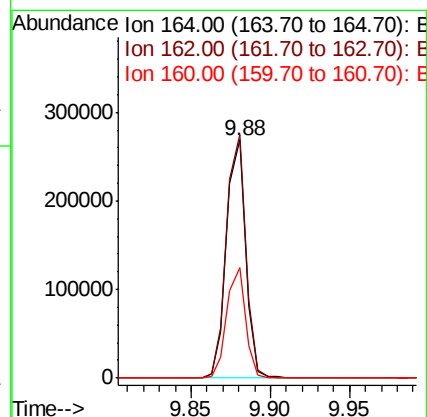




#42
 2,4,6-Tribromophenol
 Concen: 156.870 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.01 min
 Lab File: BF116715.D
 Acq: 1 Sep 2019 00:27

Instrument :
 BNA_F
 ClientSampleId :
 T9-12-13-P-(0-1.9)

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.3	76.9	115.3
141	44.1	31.4	47.2






Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

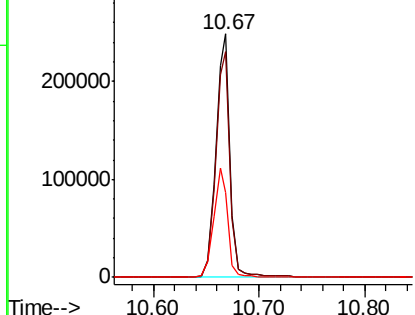

#45
 2-Fluorobiphenyl
 Concen: 94.250 ng
 RT: 9.20 min Scan# 1210
 Delta R.T. -0.00 min
 Lab File: BF116715.D
 Acq: 1 Sep 2019 00:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	27.8	41.6
170	23.9	18.9	28.3






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



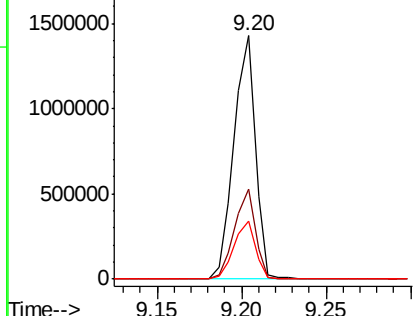





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27




Instrument :
BNA_F
ClientSampleId :
T9-12-13-P-(0-1.9)


Tot Ion:188 Resp: 375840
Ion Ratio Lower Upper
188 100
94 11.4 7.3 10.9#
80 12.5 8.4 12.6

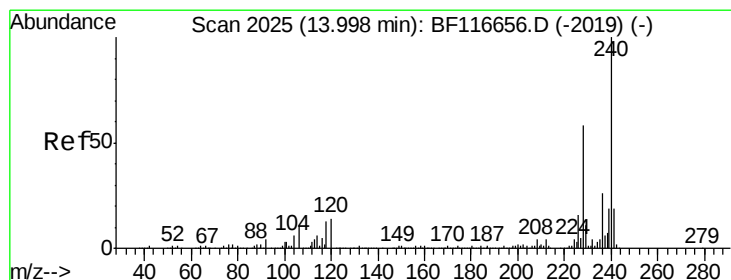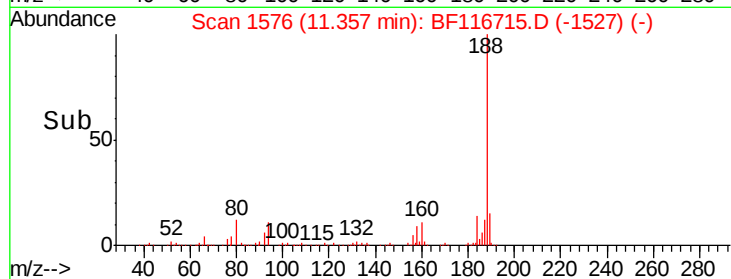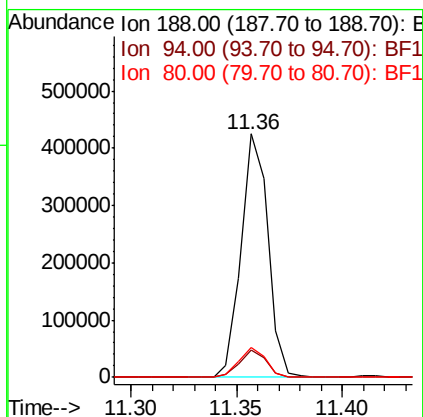

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2023
Delta R.T. -0.01 min
Lab File: BF116715.D
Acq: 1 Sep 2019 00:27

Tgt Ion:240 Resp: 248746
Ion Ratio Lower Upper
240 100
120 14.6 9.1 13.7#
236 25.8 21.1 31.7

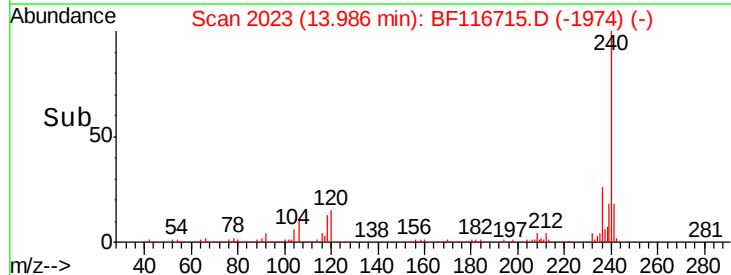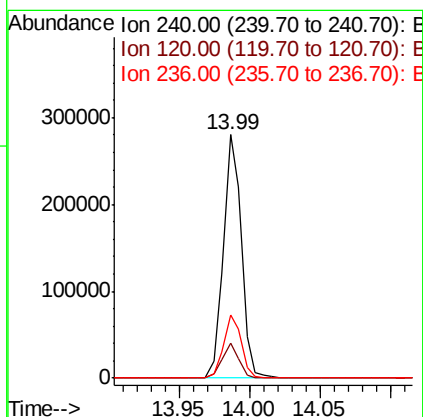



#79

Terphenyl-d14

Concen: 93.758 ng

RT: 12.94 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BF116715.D

Acq: 1 Sep 2019 00:27

Instrument :

BNA_F

ClientSampleId :

T9-12-13-P-(0-1.9)


Tot Ion:244 Resp: 1260685

Ion Ratio Lower Upper

244 100

212 7.4 6.1 9.1




122 14.3 10.2 15.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

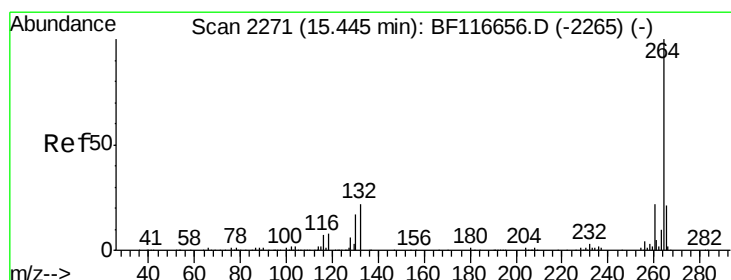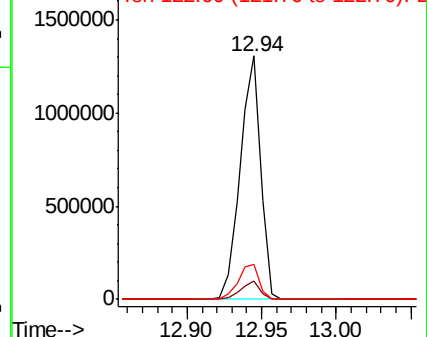

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2270

Delta R.T. -0.01 min

Lab File: BF116715.D

Acq: 1 Sep 2019 00:27


Tgt Ion:264 Resp: 276236

Ion Ratio Lower Upper

264 100

260 23.0 18.3 27.5

265 22.2 16.5 24.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

