


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083119\
 Data File : BF116687.D
 Acq On : 31 Aug 2019 9:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

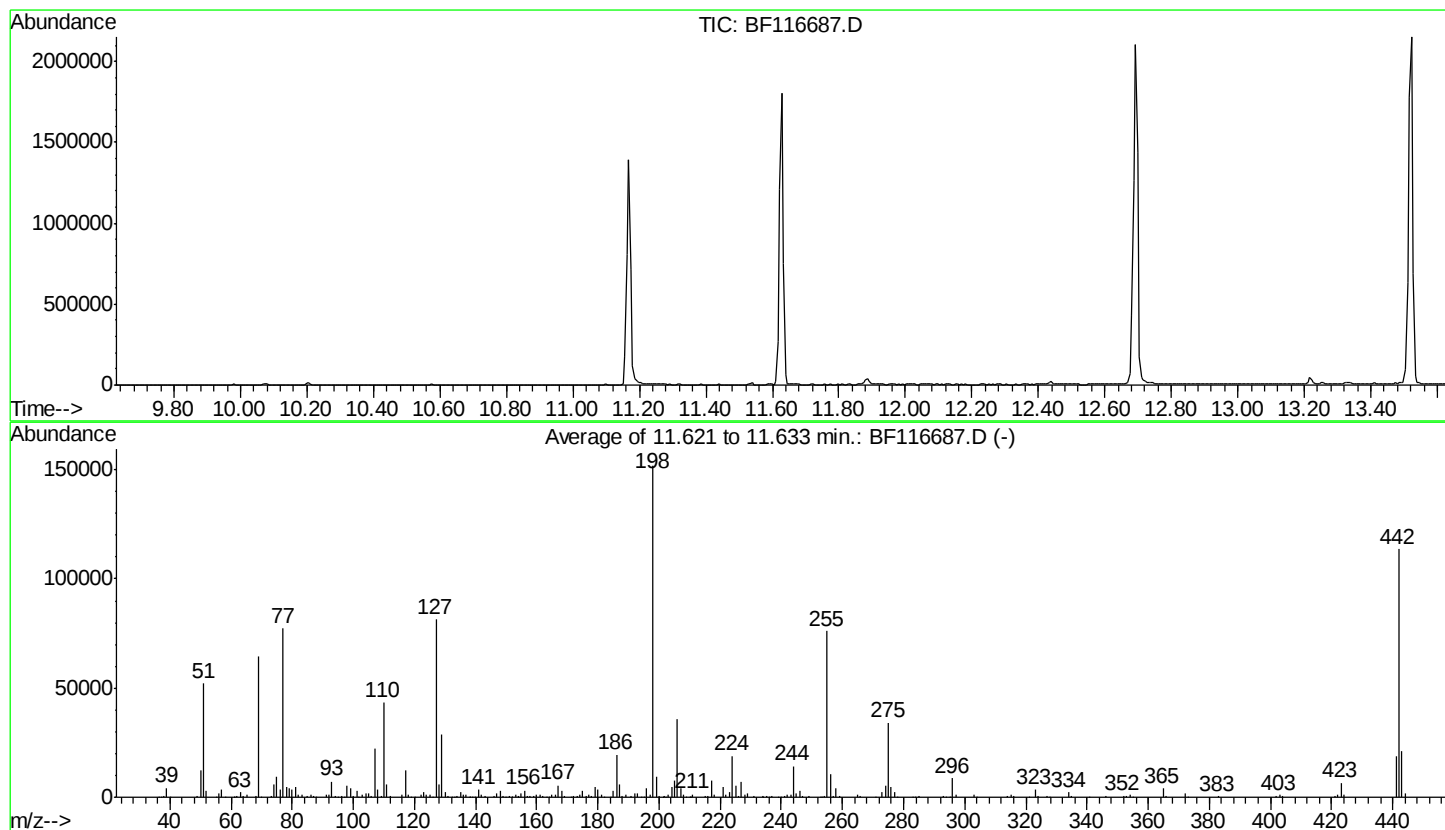

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	52149	PASS
68	69	0.00	2	1.3	807	PASS
69	198	0.00	100	42.3	64306	PASS
70	69	0.00	2	0.1	48	PASS
127	198	10	80	53.5	81261	PASS
197	198	0.00	2	0.8	1152	PASS
198	198	100	100	100.0	151874	PASS
199	198	5	9	6.4	9674	PASS
275	198	10	60	22.5	34144	PASS
365	198	1	100	2.6	3899	PASS
441	198	0.01	100	12.3	18696	PASS
442	198	50	100	74.8	113613	PASS
443	442	15	24	18.7	21248	PASS