
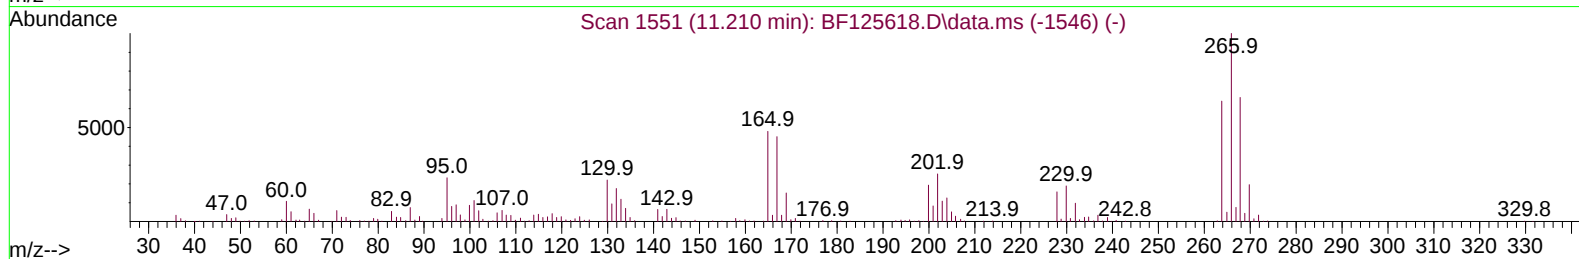
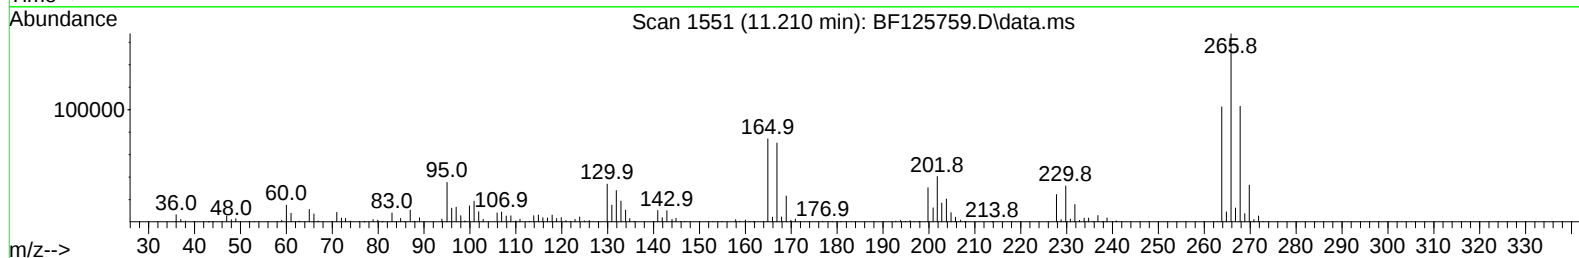


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125759.D
Acq On : 4 Oct 2021 11:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 13:40:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

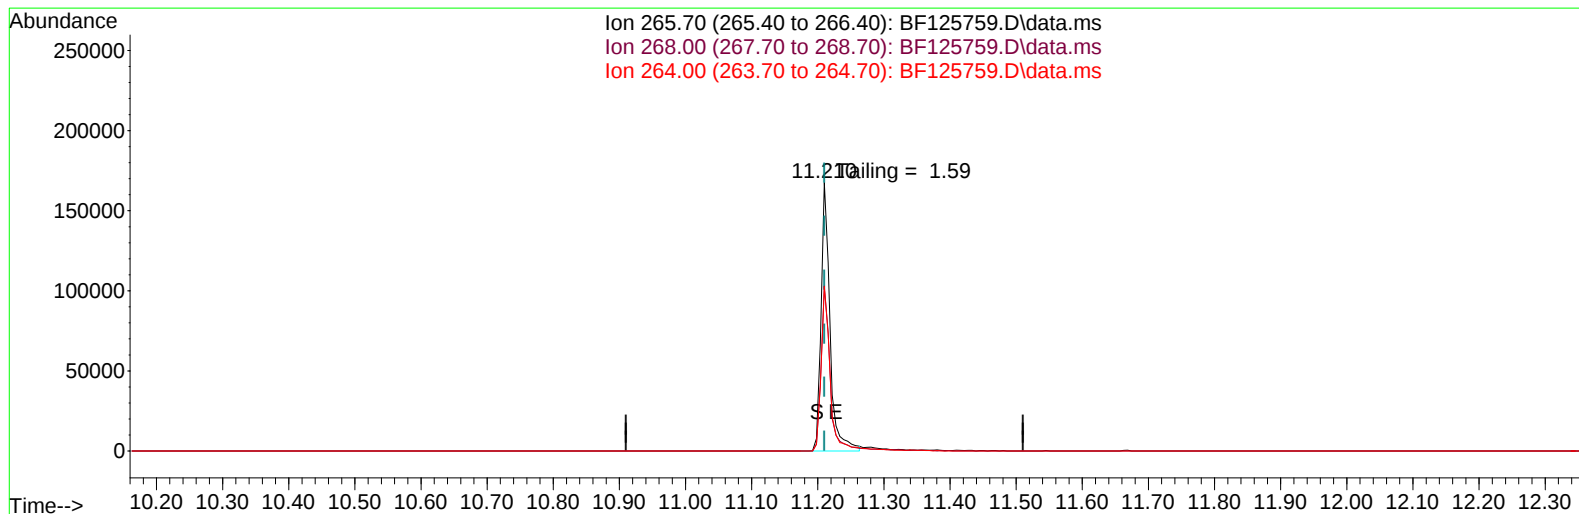

TIC: BF125759.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 33245.99 ng

response 163618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.48
264.00	69.90	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125759.D
Acq On : 4 Oct 2021 11:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 13:40:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

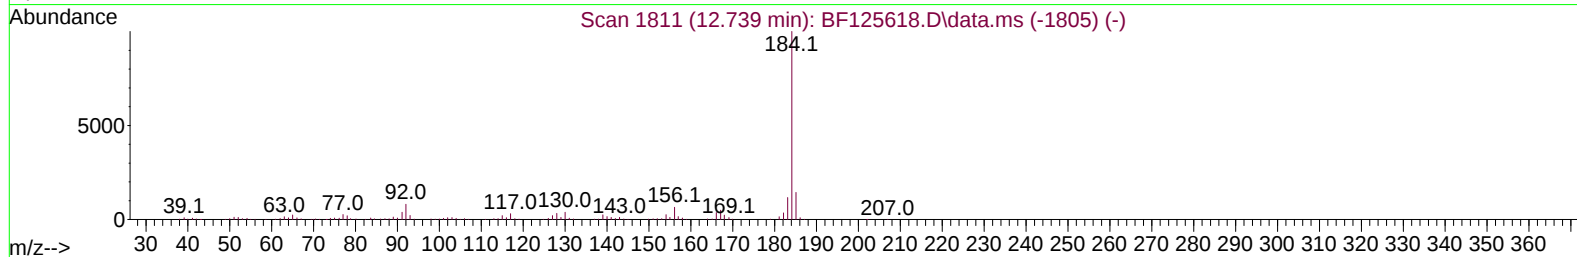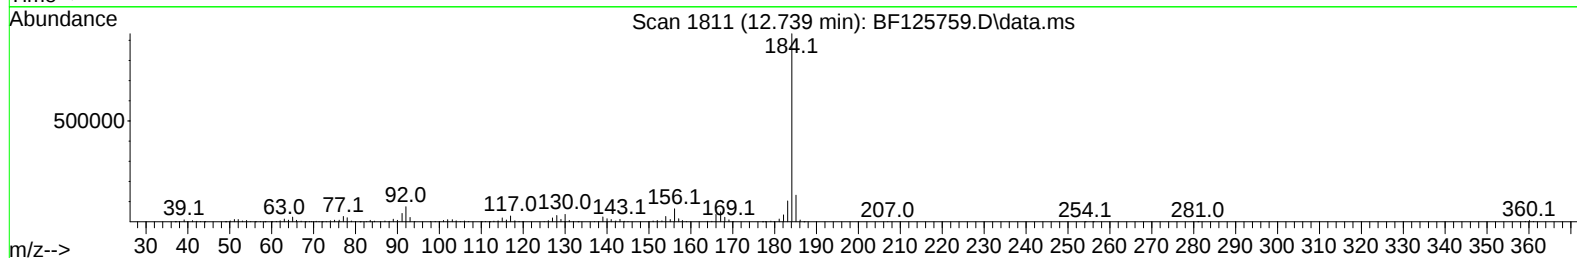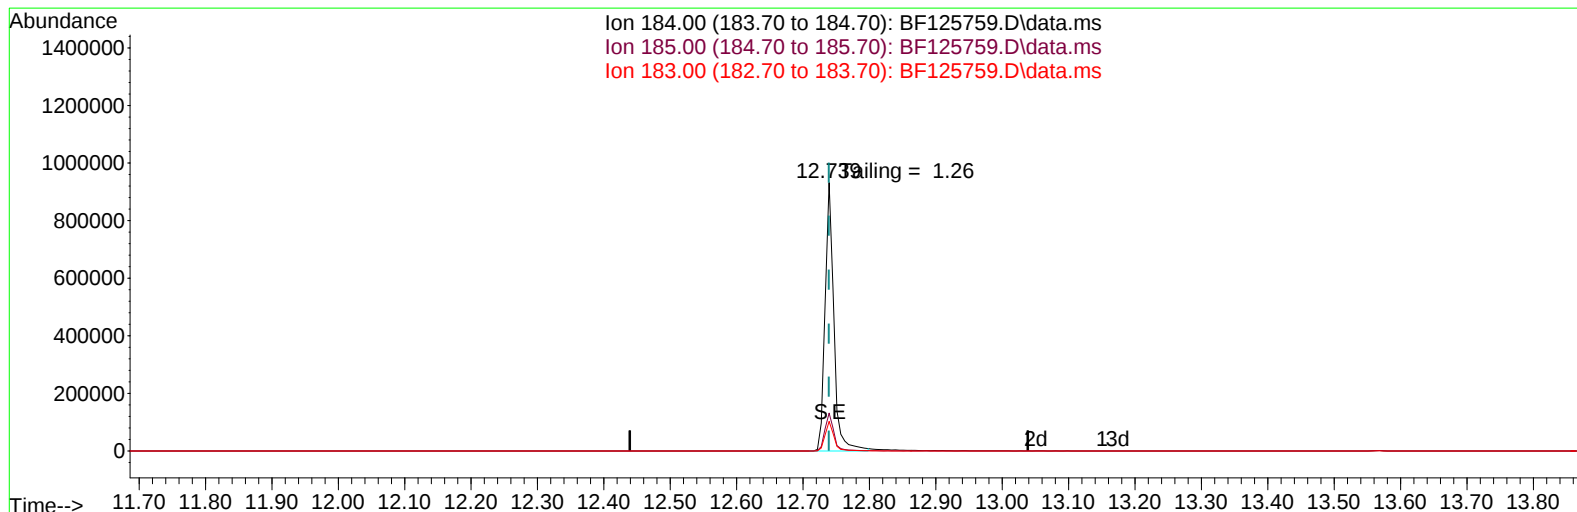

TIC: BF125759.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 236691.20 ng m

response 876730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.15
183.00	10.10	11.08
0.00	0.00	0.00