

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
 Data File : BF125762.D
 Acq On : 4 Oct 2021 12:45
 Operator : JU/CG
 Sample : PB139583BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139583BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.252	19	28	35	rVB	119743	153253	2.41%	0.395%
2	2.357	40	46	52	rBV	79825	100225	1.58%	0.258%
3	5.140	515	519	528	rVB	55522	74496	1.17%	0.192%
4	5.516	577	583	586	rBV	4843415	5393805	84.81%	13.888%
5	6.516	746	753	755	rBV	4232089	5294266	83.25%	13.631%
6	6.887	812	816	820	rBV	1547529	1229650	19.33%	3.166%
7	7.451	906	912	915	rBV	3309029	3449500	54.24%	8.882%
8	8.169	1029	1034	1037	rBV	1936020	1659650	26.10%	4.273%
9	9.245	1211	1217	1220	rBV	6549541	6359744	100.00%	16.375%
10	9.922	1327	1332	1347	rBV	2074563	1832869	28.82%	4.719%
11	10.710	1462	1466	1479	rBV	3738080	3514440	55.26%	9.049%
12	11.410	1581	1585	1588	rBV	1889998	1697875	26.70%	4.372%
13	12.992	1850	1854	1858	rBV	5622543	5695973	89.56%	14.666%
14	14.045	2029	2033	2042	rBV	1265779	1272730	20.01%	3.277%
15	15.521	2278	2284	2297	rBV	829785	1110409	17.46%	2.859%




Sum of corrected areas: 38838885

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125762.D
Acq On : 4 Oct 2021 12:45
Operator : JU/CG
Sample : PB139583BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139583BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

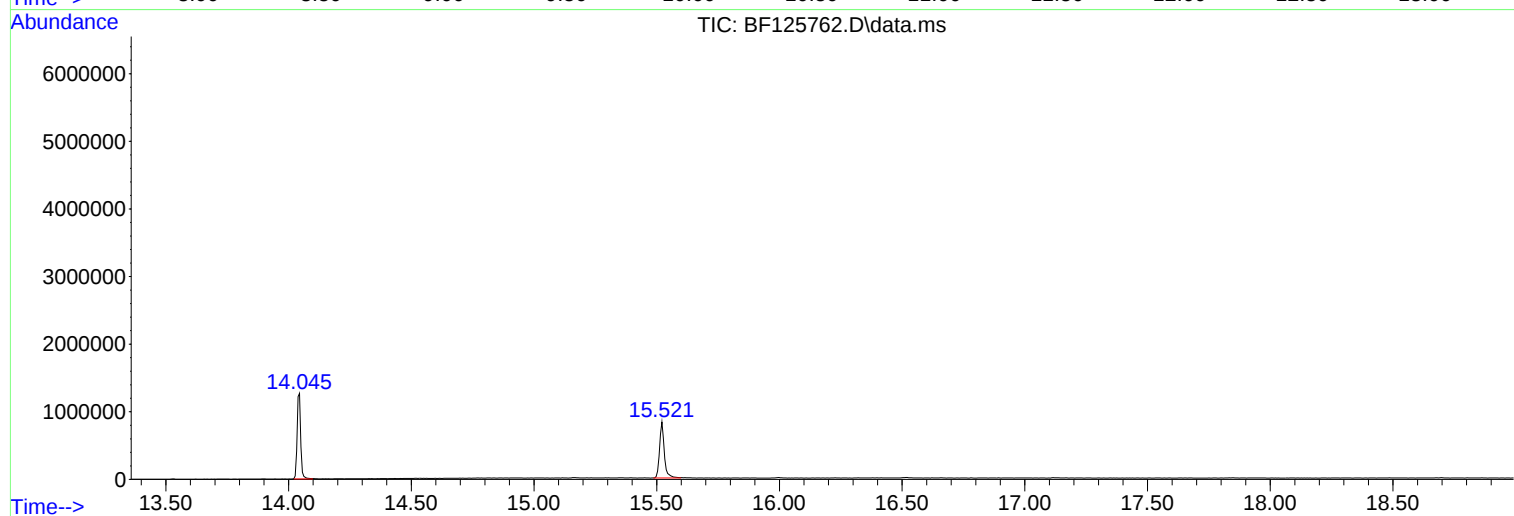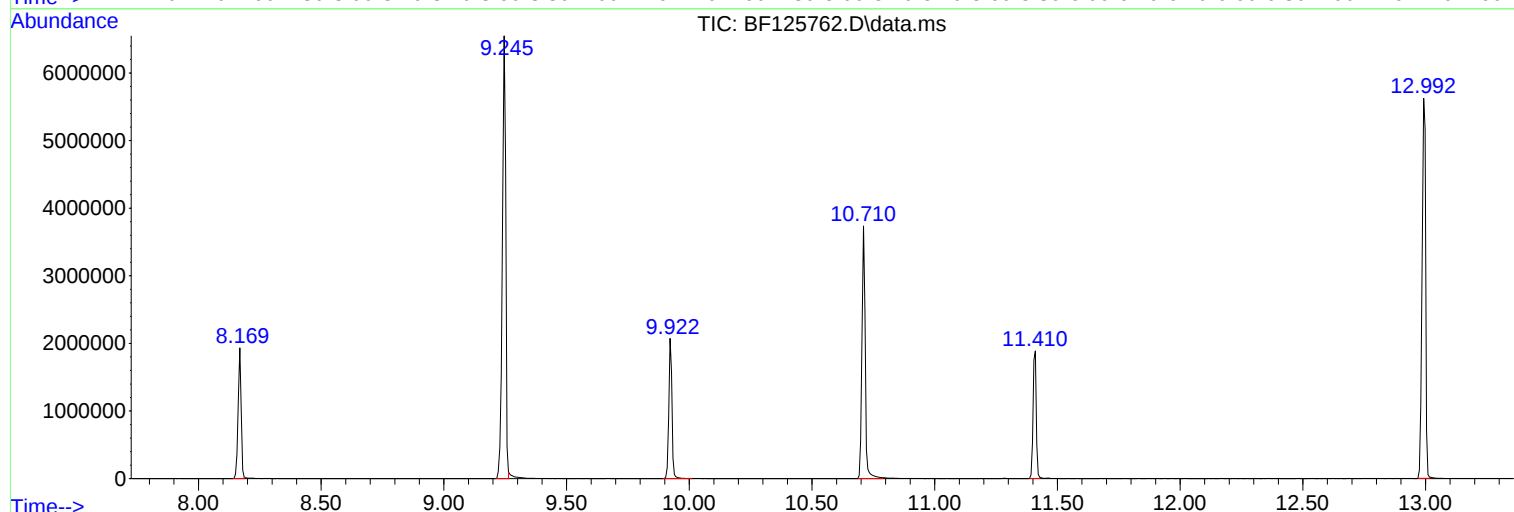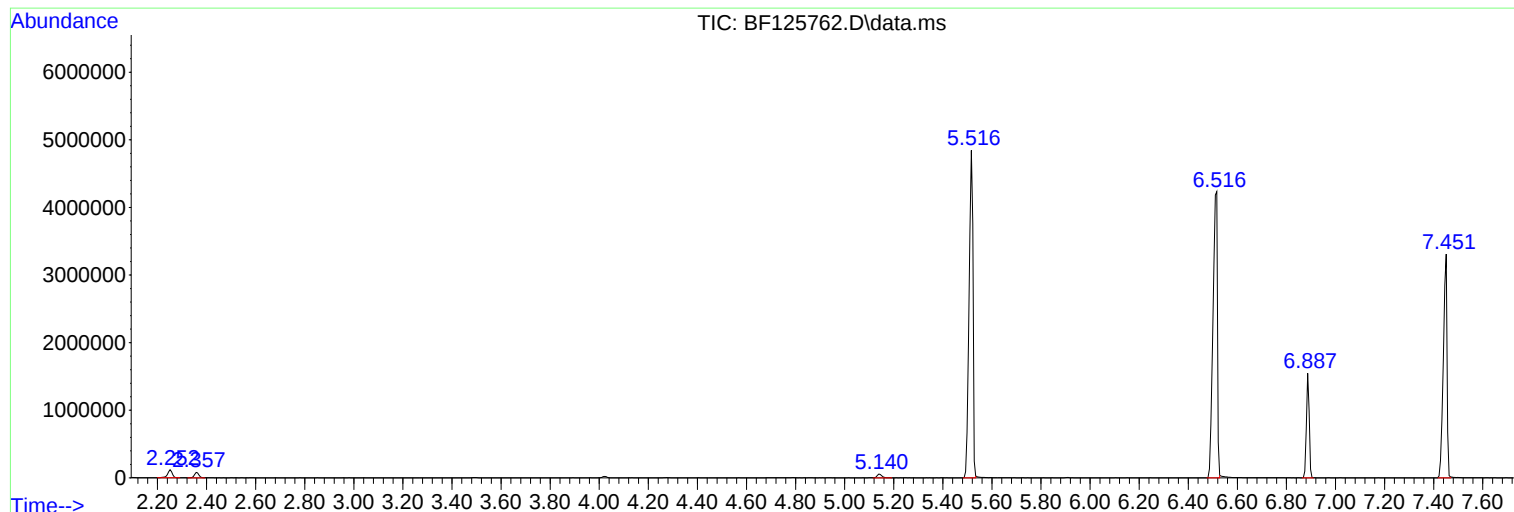

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125762.D
Acq On : 4 Oct 2021 12:45
Operator : JU/CG
Sample : PB139583BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139583BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.252	2.49 ng	153253	1,4-Dichlorobenzene-d4	6.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	10

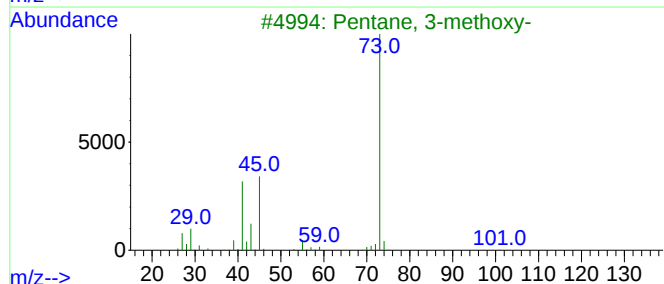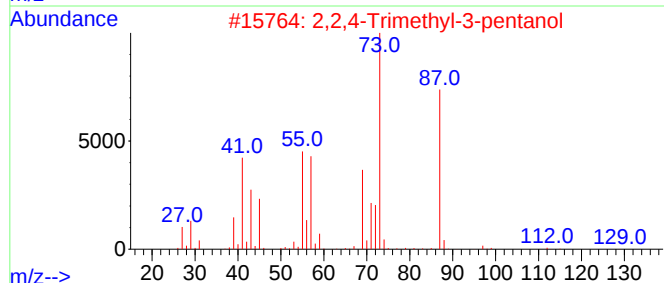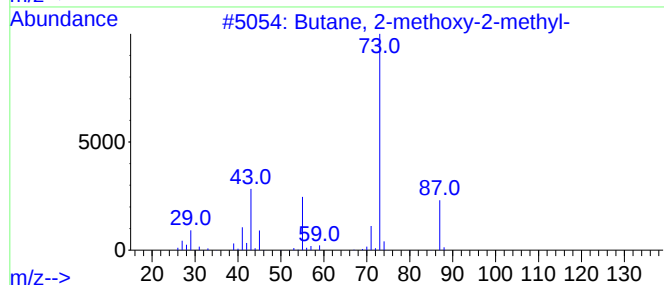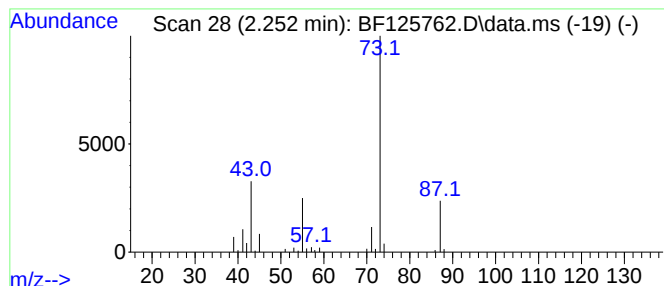

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125762.D
Acq On : 4 Oct 2021 12:45
Operator : JU/CG
Sample : PB139583BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139583BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.252	2.5	ng	153253	1	6.887	1229650	20.0