


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
 Data File : BF125759.D
 Acq On : 4 Oct 2021 11:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

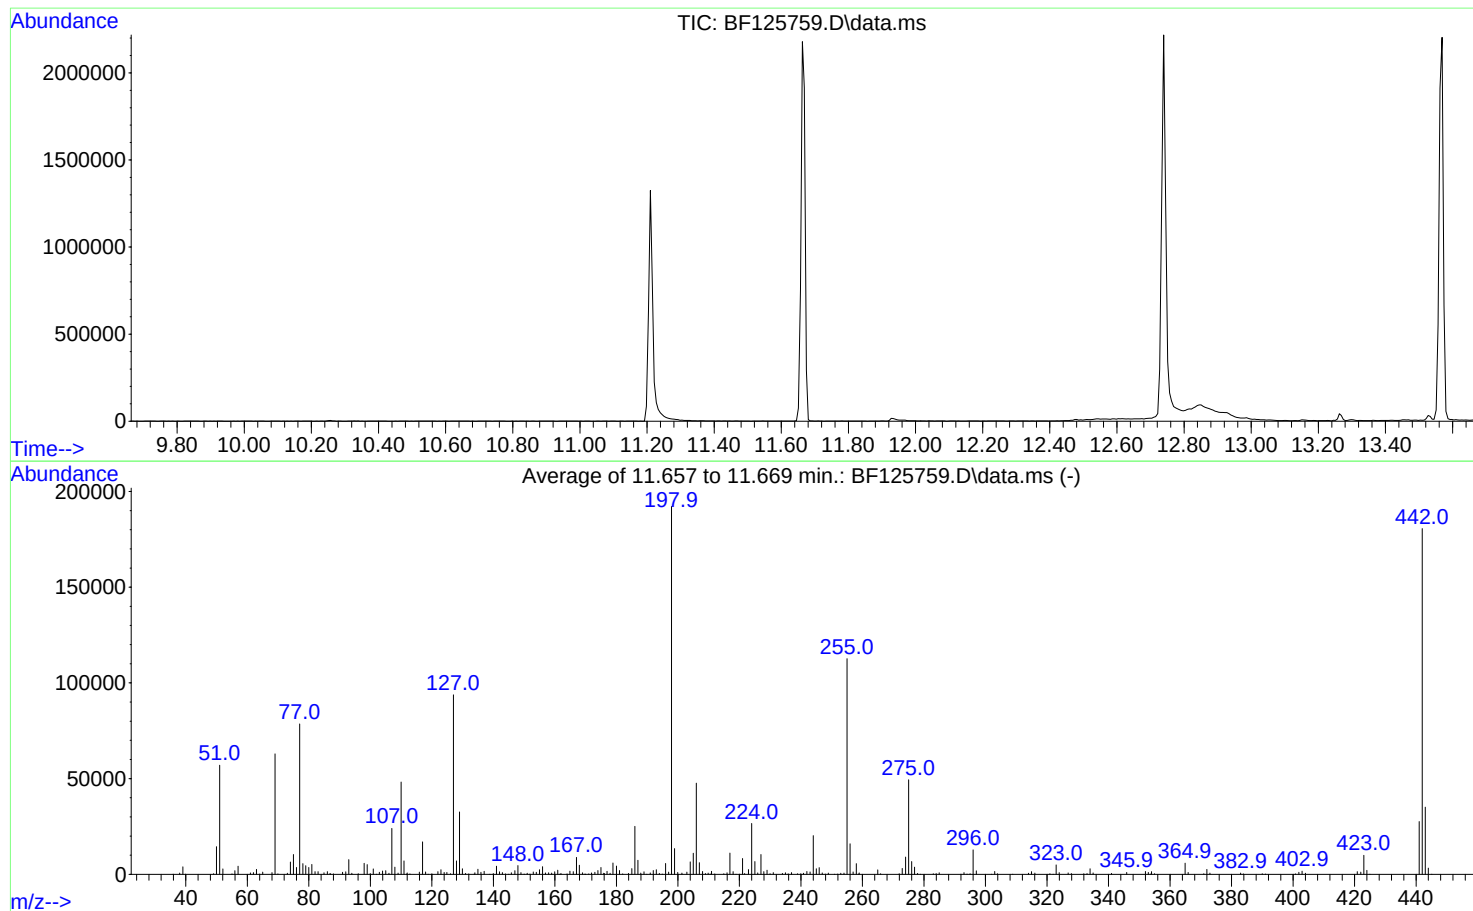




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	56997	PASS
68	69	0.00	2	1.5	916	PASS
69	198	0.00	100	32.8	62947	PASS
70	69	0.00	2	0.4	249	PASS
127	198	10	80	48.8	93789	PASS
197	198	0.00	2	0.6	1174	PASS
198	198	100	100	100.0	192139	PASS
199	198	5	9	7.0	13459	PASS
275	198	10	60	25.7	49419	PASS
365	198	1	100	3.1	5871	PASS
441	198	0.01	100	14.3	27544	PASS
442	442	50	100	100.0	180645	PASS
443	442	15	24	19.4	35067	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
 Data File : BF125759.D
 Acq On : 4 Oct 2021 11:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 13:40:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

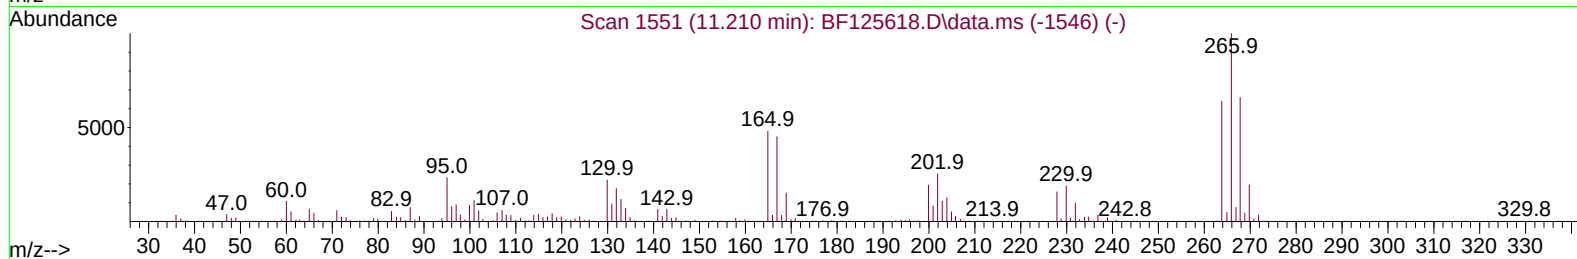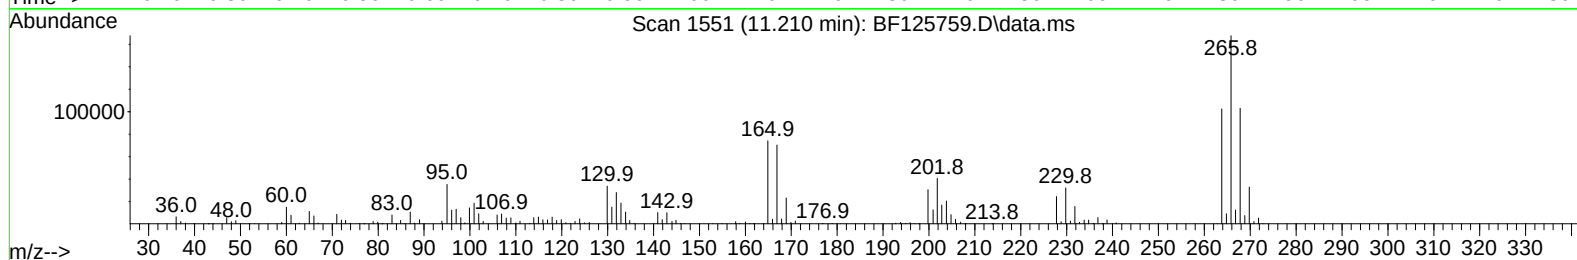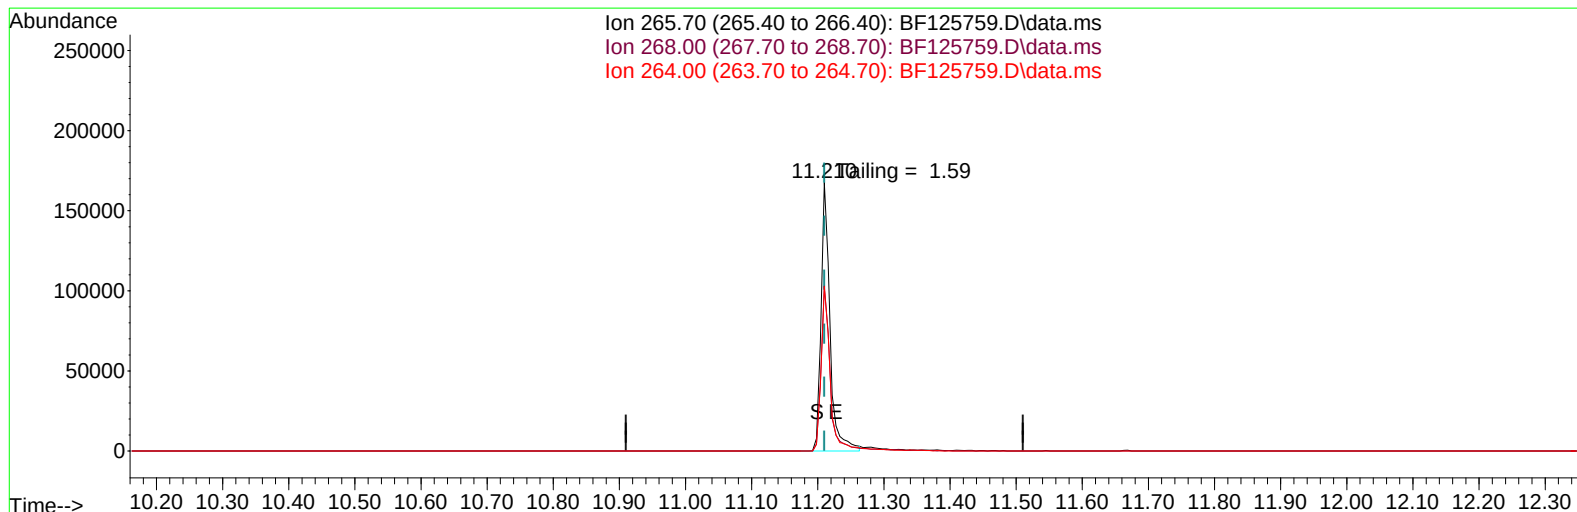

TIC: BF125759.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 33245.99 ng




response 163618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.48
264.00	69.90	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100421\
Data File : BF125759.D
Acq On : 4 Oct 2021 11:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 13:40:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

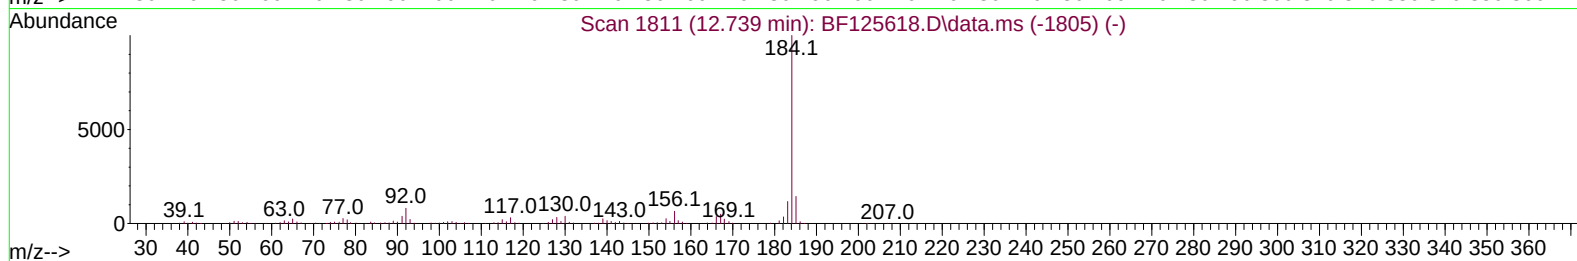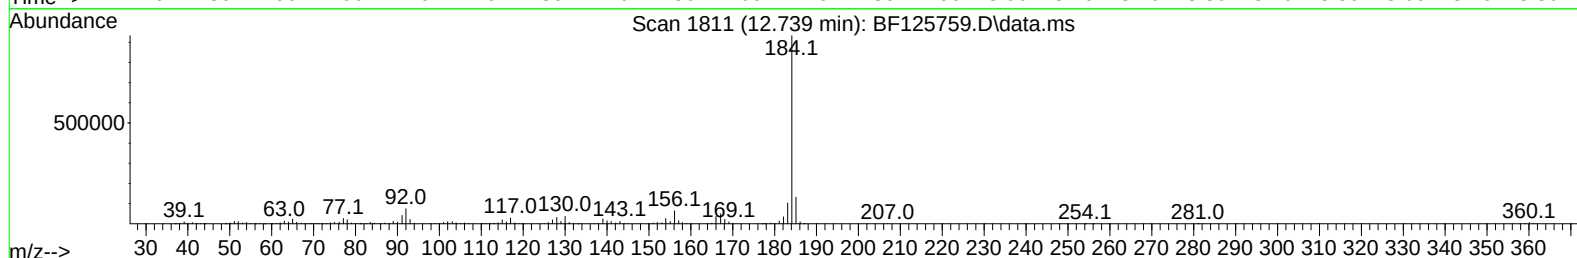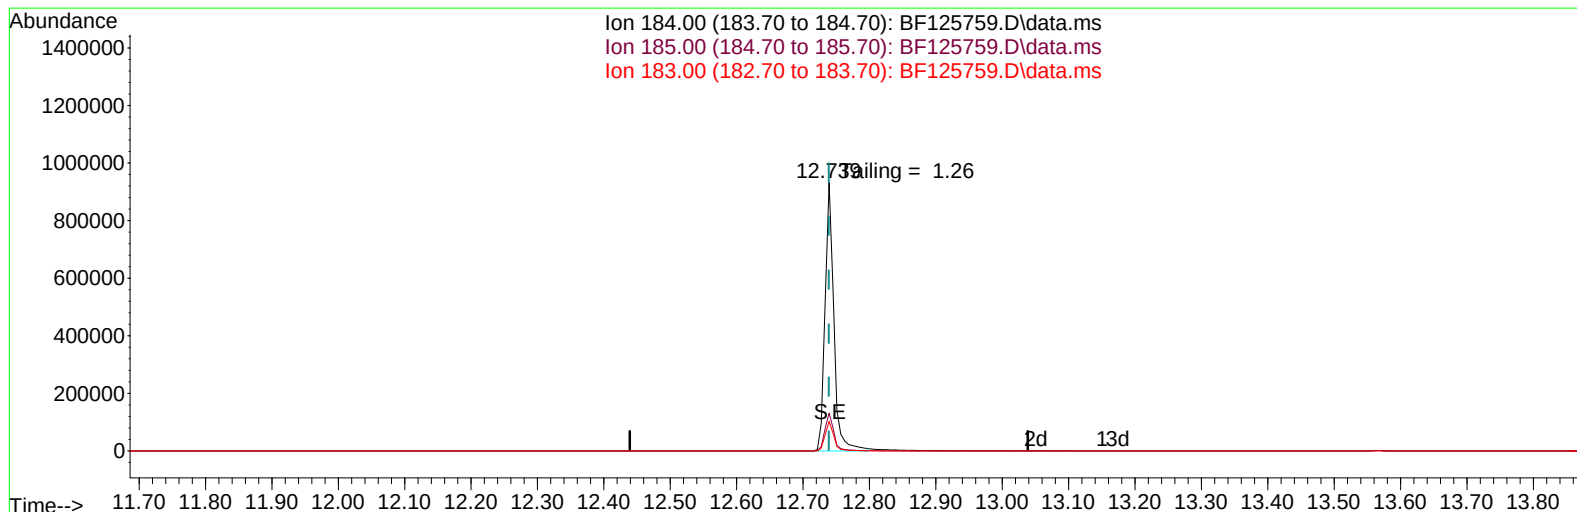

TIC: BF125759.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 236691.20 ng m

response 876730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.15
183.00	10.10	11.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_F	<u>BF125759.D</u>
Compound Name	Response	Retention Time
DDT	371441	13.56
DDD	7224	13.26
DDE	1459	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8683	380124	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP