
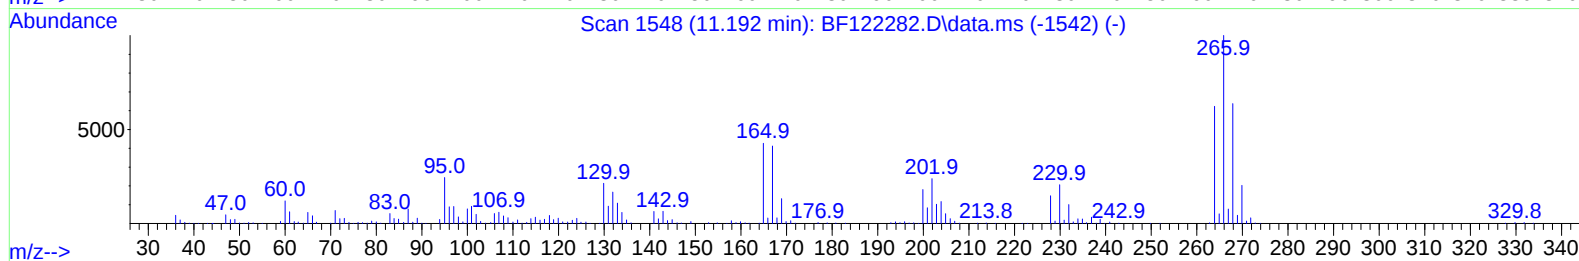
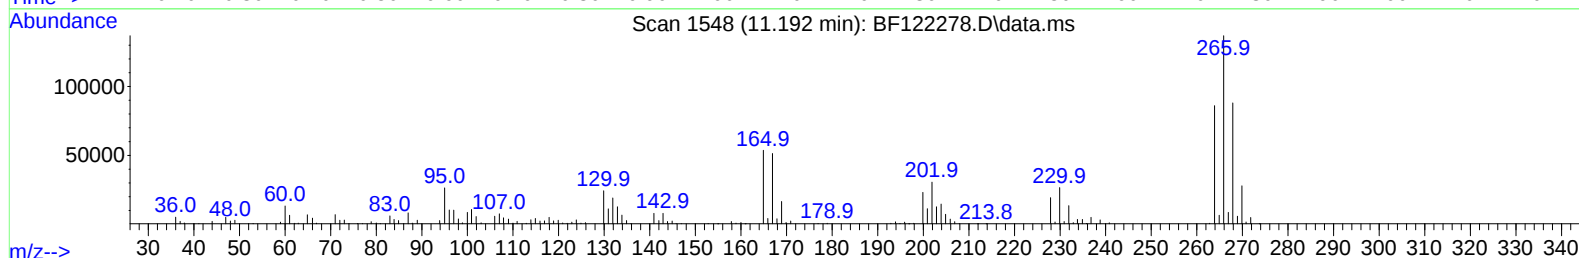


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110920\
Data File : BF122278.D
Acq On : 9 Nov 2020 10:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:47:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 09 15:51:40 2020
Response via : Initial Calibration

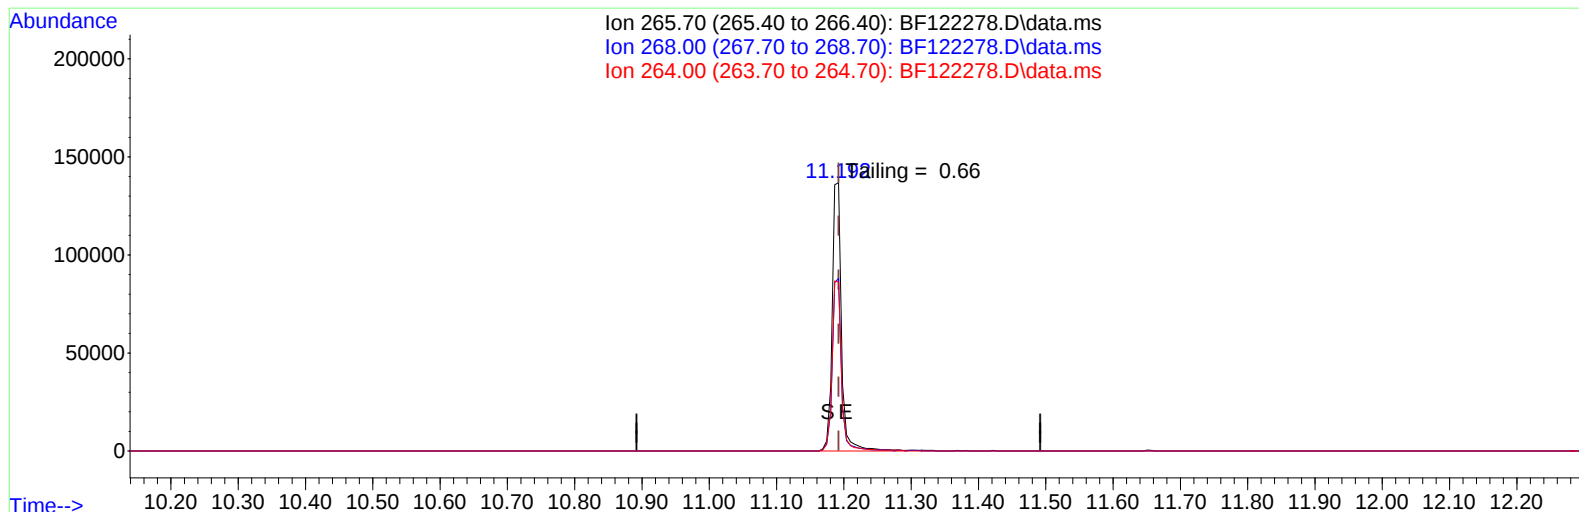

TIC: BF122278.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 22334.68 ng

response 132168

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.34
264.00	62.40	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110920\
Data File : BF122278.D
Acq On : 9 Nov 2020 10:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:47:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 09 15:51:40 2020
Response via : Initial Calibration

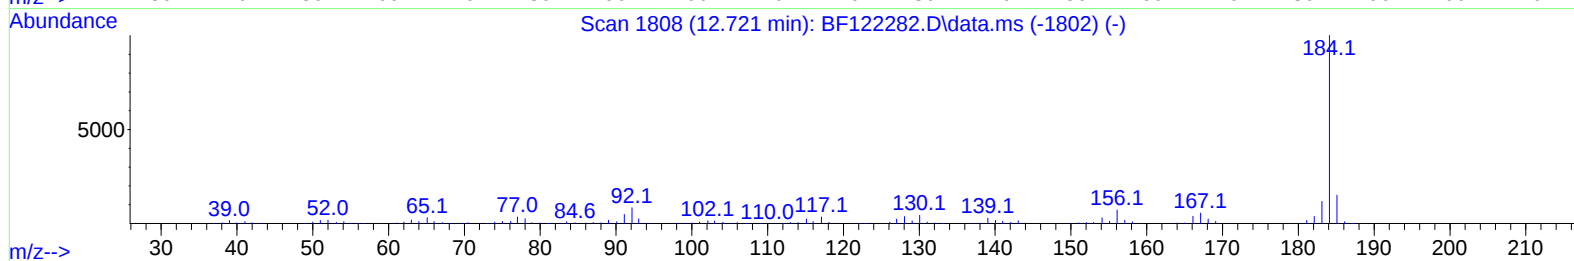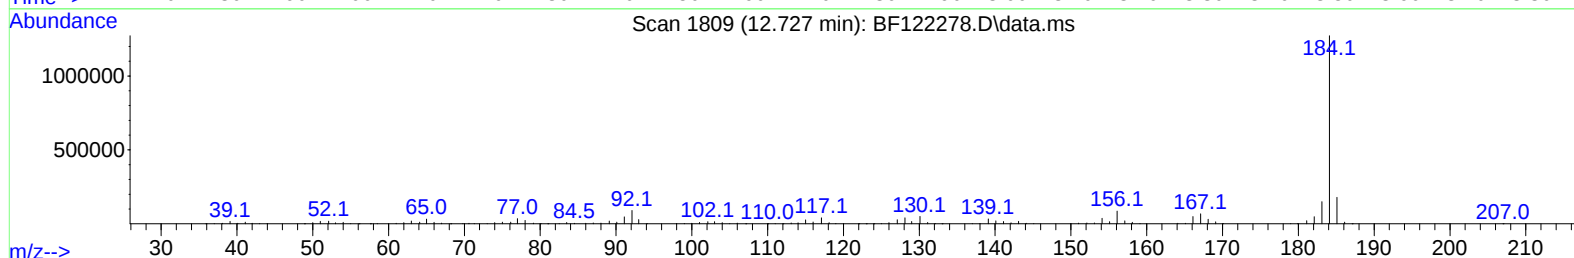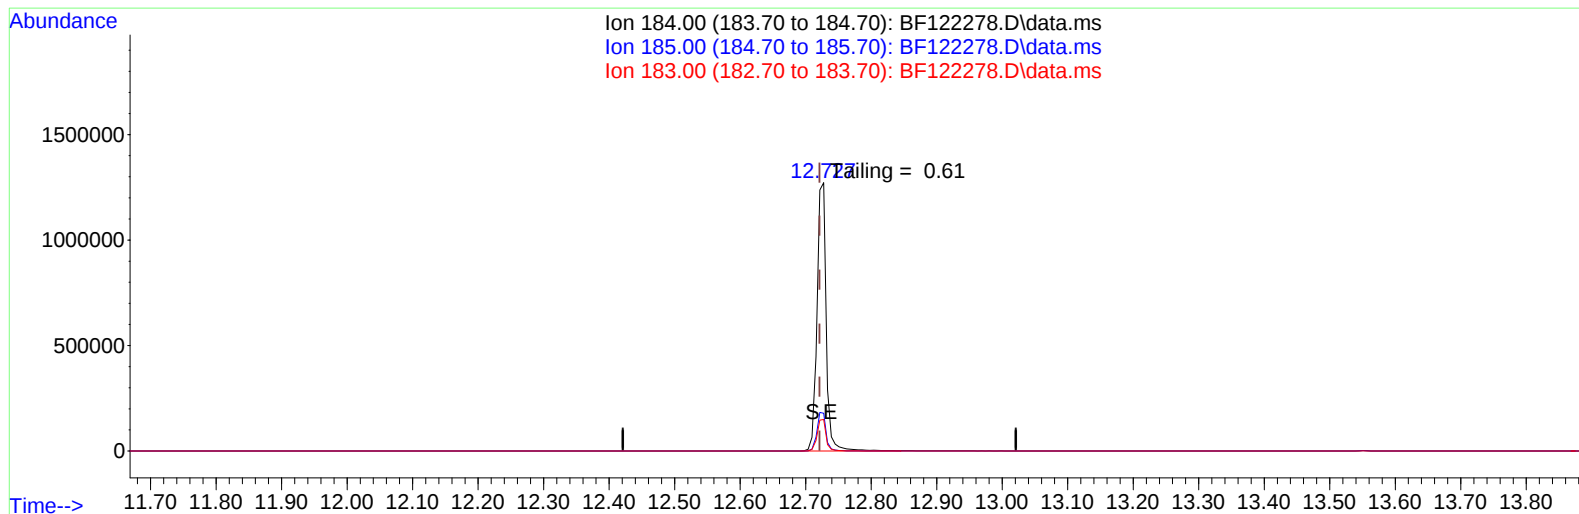

TIC: BF122278.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 1246390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.07
183.00	11.70	11.75
0.00	0.00	0.00