


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110920\
Data File : BF122278.D
Acq On : 9 Nov 2020 10:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 09 15:51:40 2020

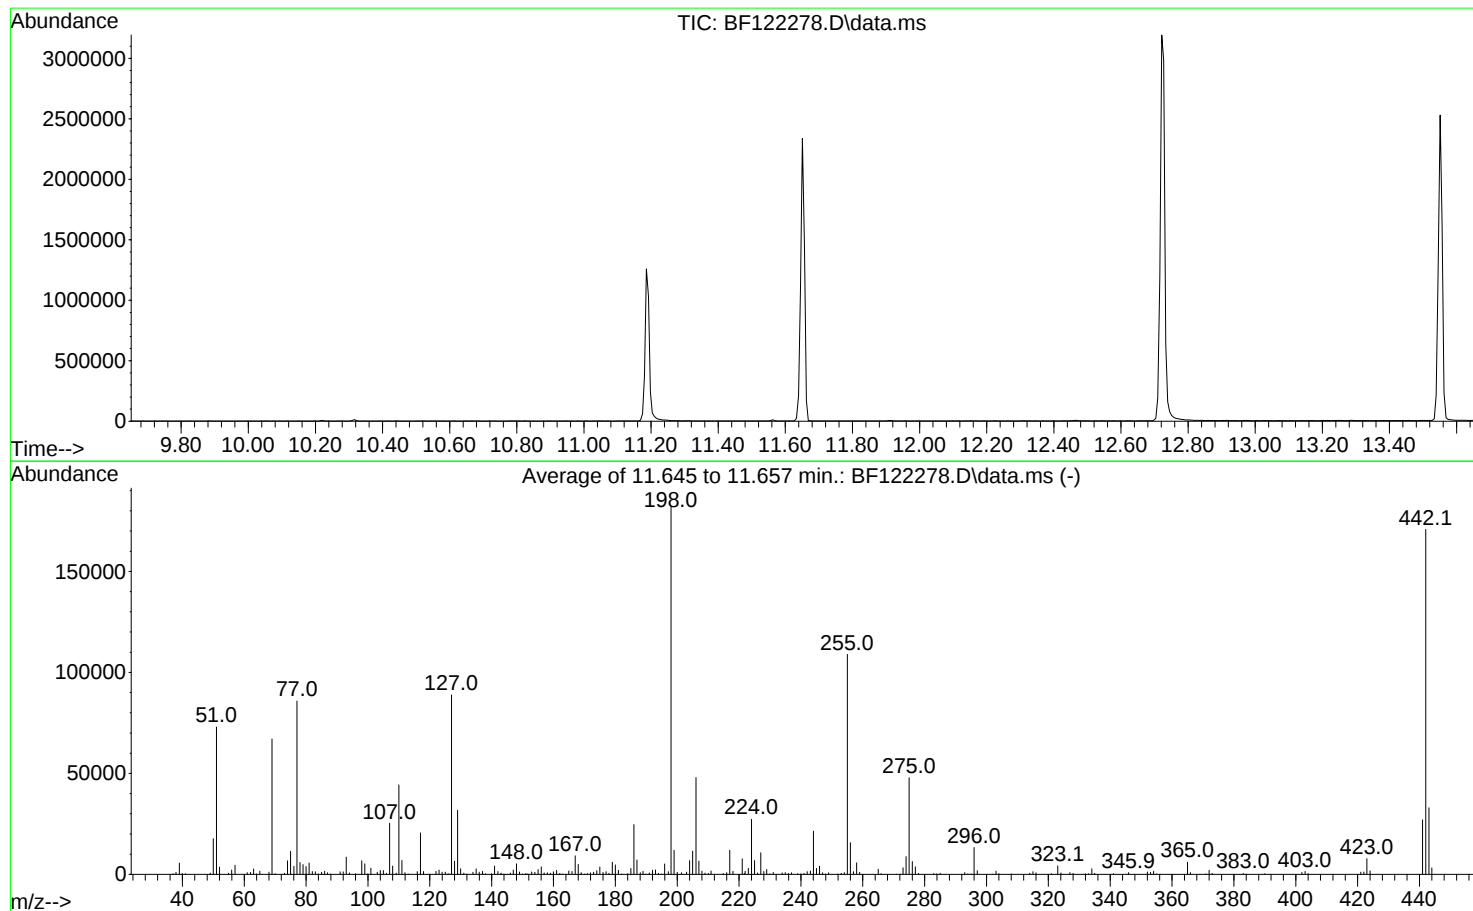

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	72949	PASS
68	69	0.00	2	1.6	1081	PASS
69	198	0.00	100	36.8	67051	PASS
70	69	0.00	2	0.5	309	PASS
127	198	10	80	48.8	88827	PASS
197	198	0.00	2	0.7	1354	PASS
198	198	100	100	100.0	182155	PASS
199	198	5	9	6.5	11911	PASS
275	198	10	60	26.3	47835	PASS
365	198	1	100	3.3	5944	PASS
441	198	0.01	100	14.8	27016	PASS
442	198	50	100	93.8	170789	PASS
443	442	15	24	19.3	32958	PASS