
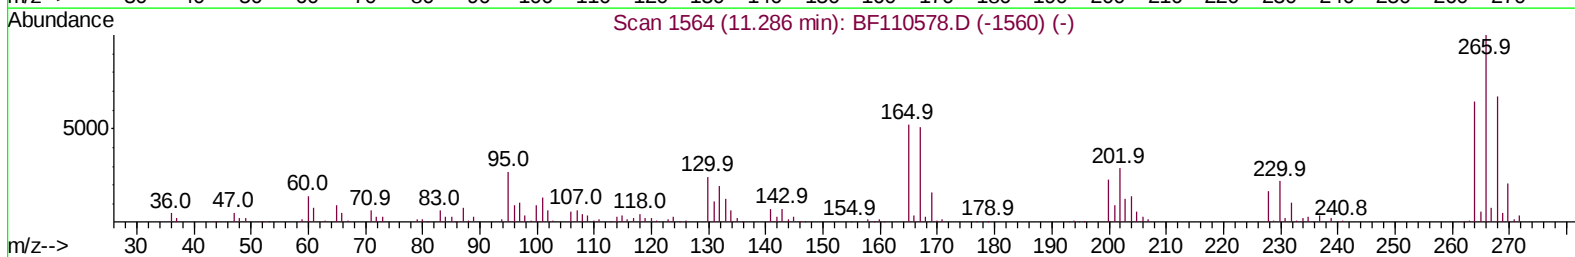
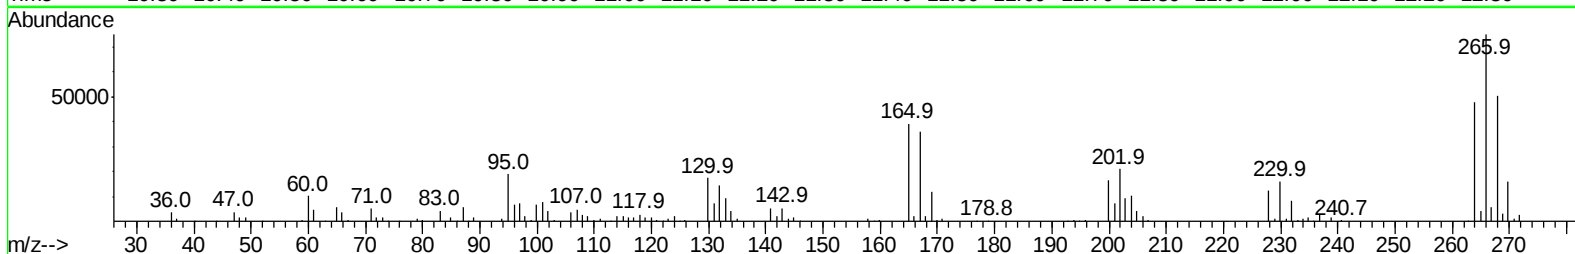


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112618\
Data File : BF110951.D
Acq On : 26 Nov 2018 9:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 10:13:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

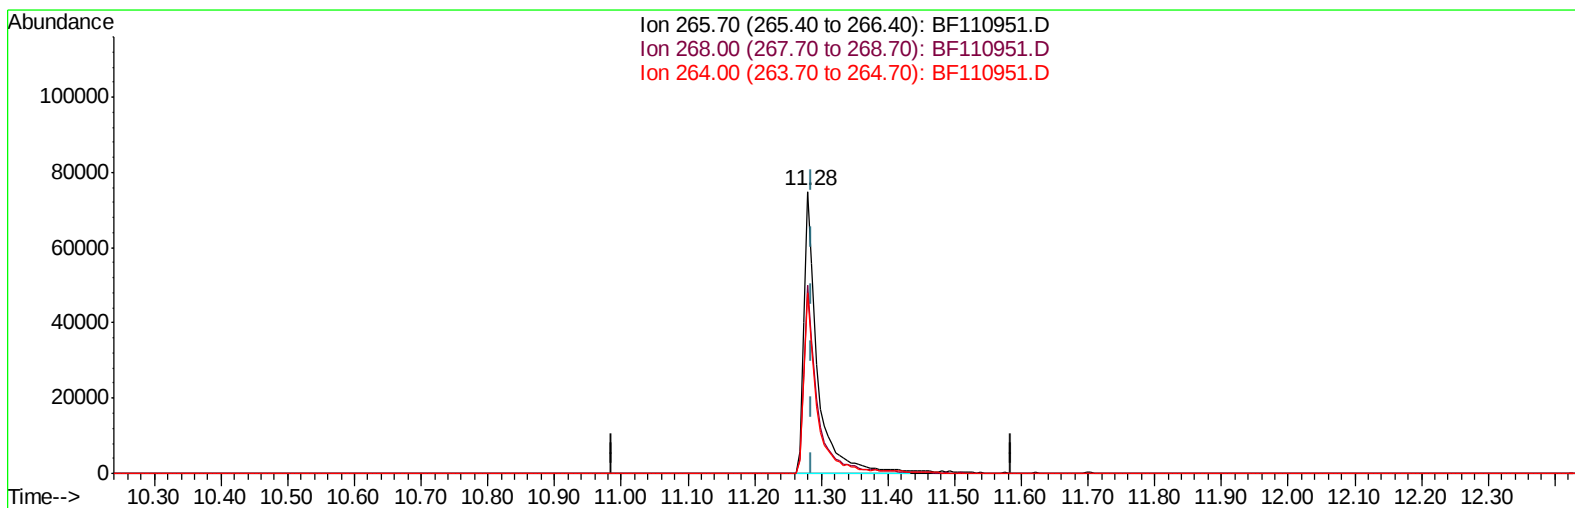

TIC: BF110951.D

(70) Pentachlorophenol (C)




11.280min (-0.006) 0.00ng

response 103441

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	66.99
264.00	63.20	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112618\
 Data File : BF110951.D
 Acq On : 26 Nov 2018 9:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 10:13:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration

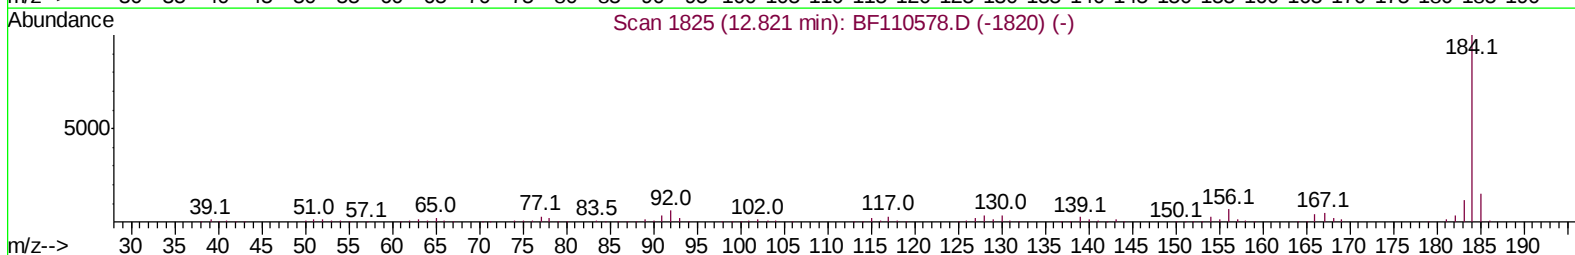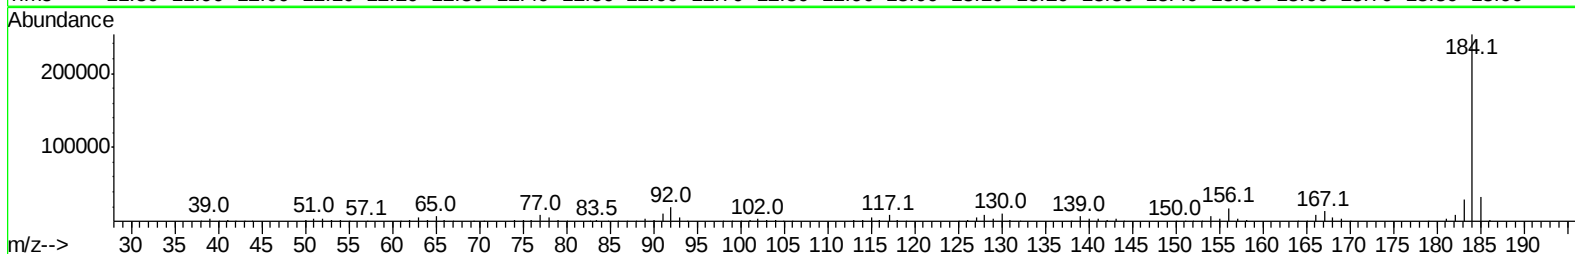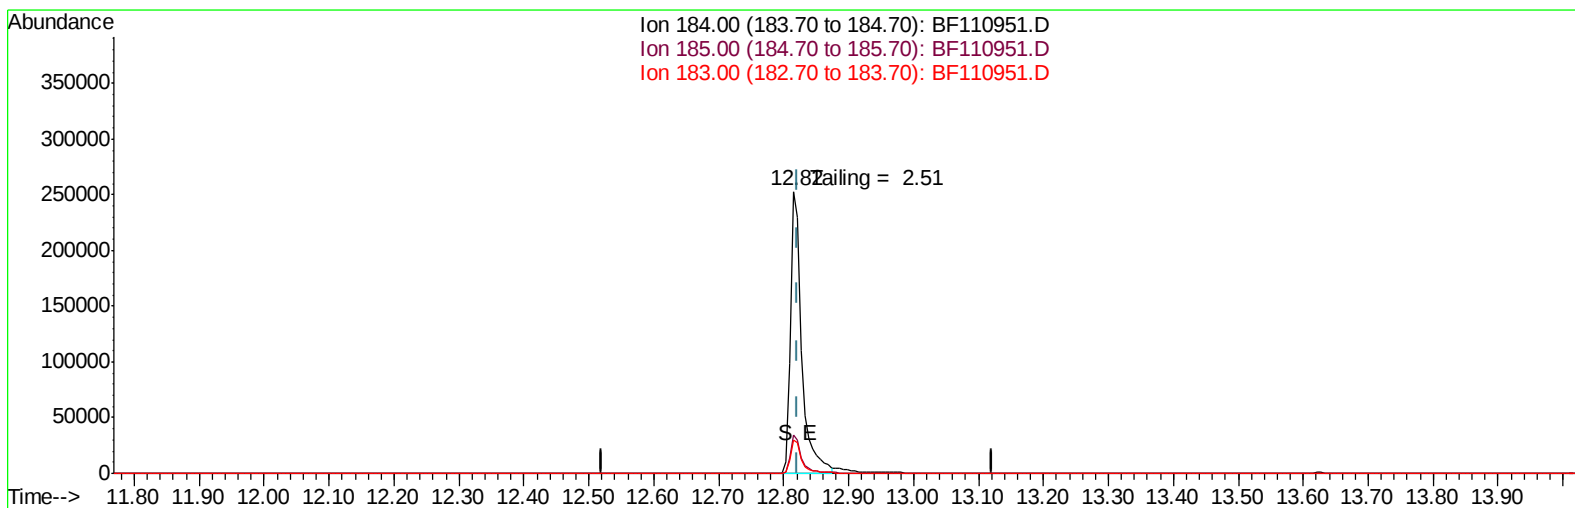

TIC: BF110951.D

(77) Benzidine

12.815min (-0.006) 0.00ng

response 314658

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	13.47
183.00	11.80	11.70
0.00	0.00	0.00