
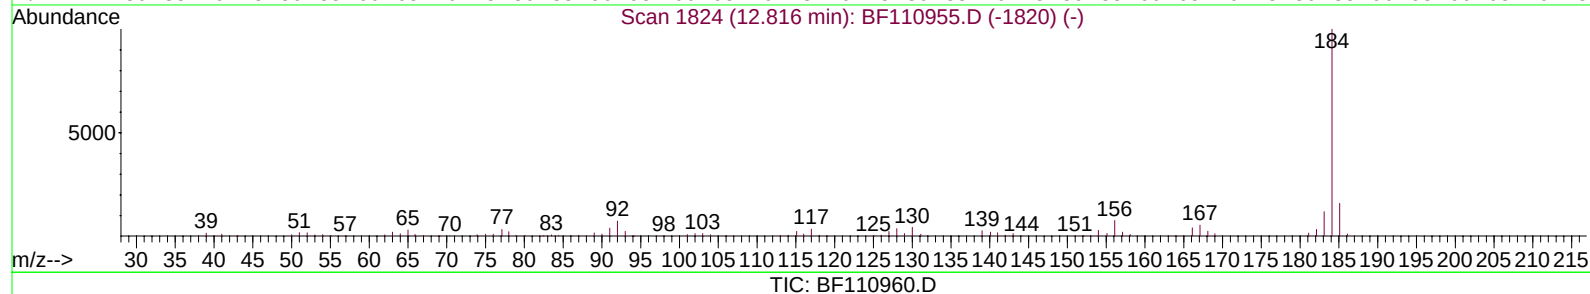
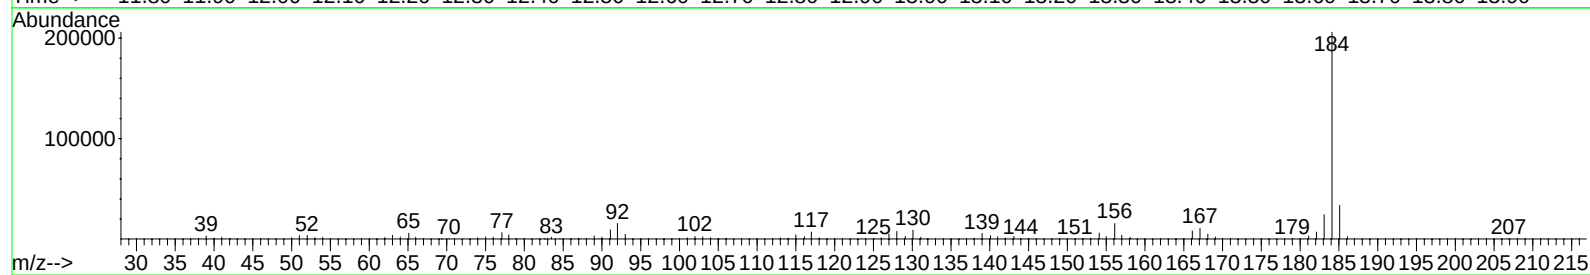


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112618\
Data File : BF110960.D
Acq On : 26 Nov 2018 13:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 14:33:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 26 14:02:09 2018
Response via : Initial Calibration

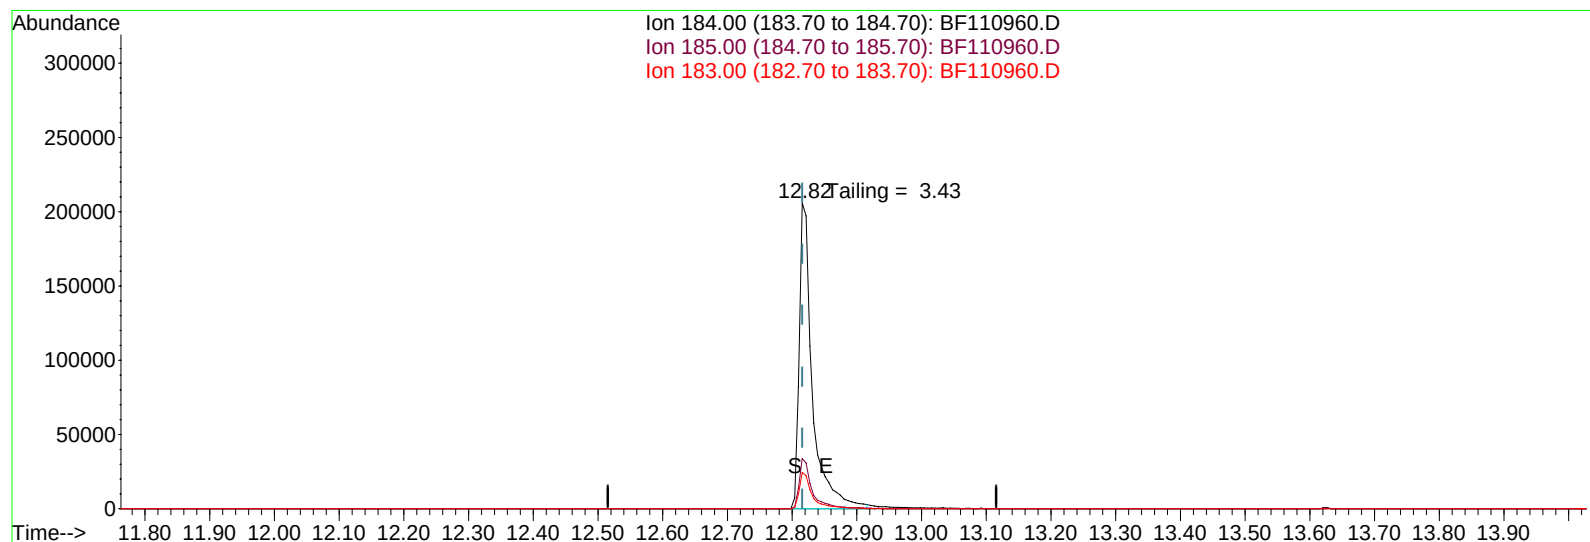

(77) Benzidine




12.816min (+0.000) 0.00ng

response 298360

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.42
183.00	11.80	11.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112618\
Data File : BF110960.D
Acq On : 26 Nov 2018 13:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 14:33:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 26 14:02:09 2018
Response via : Initial Calibration

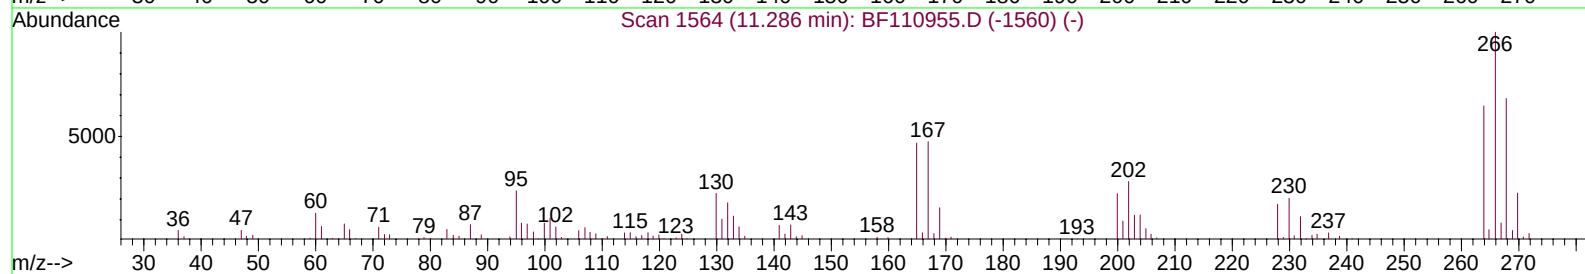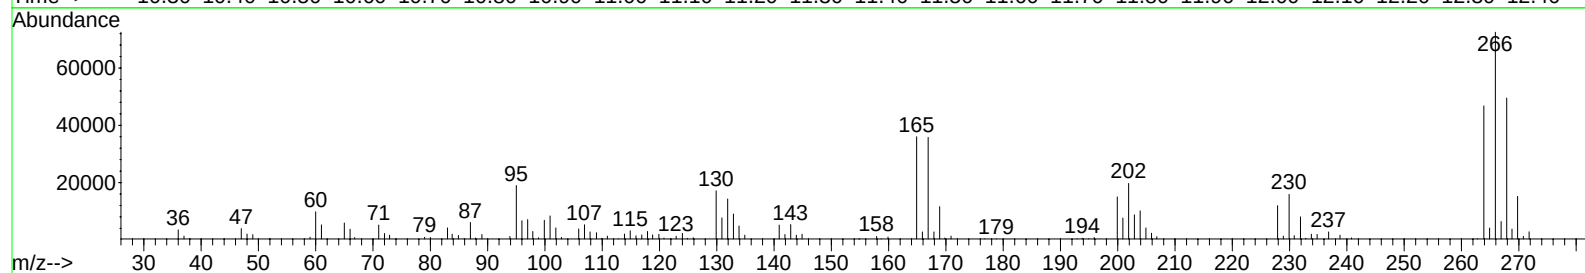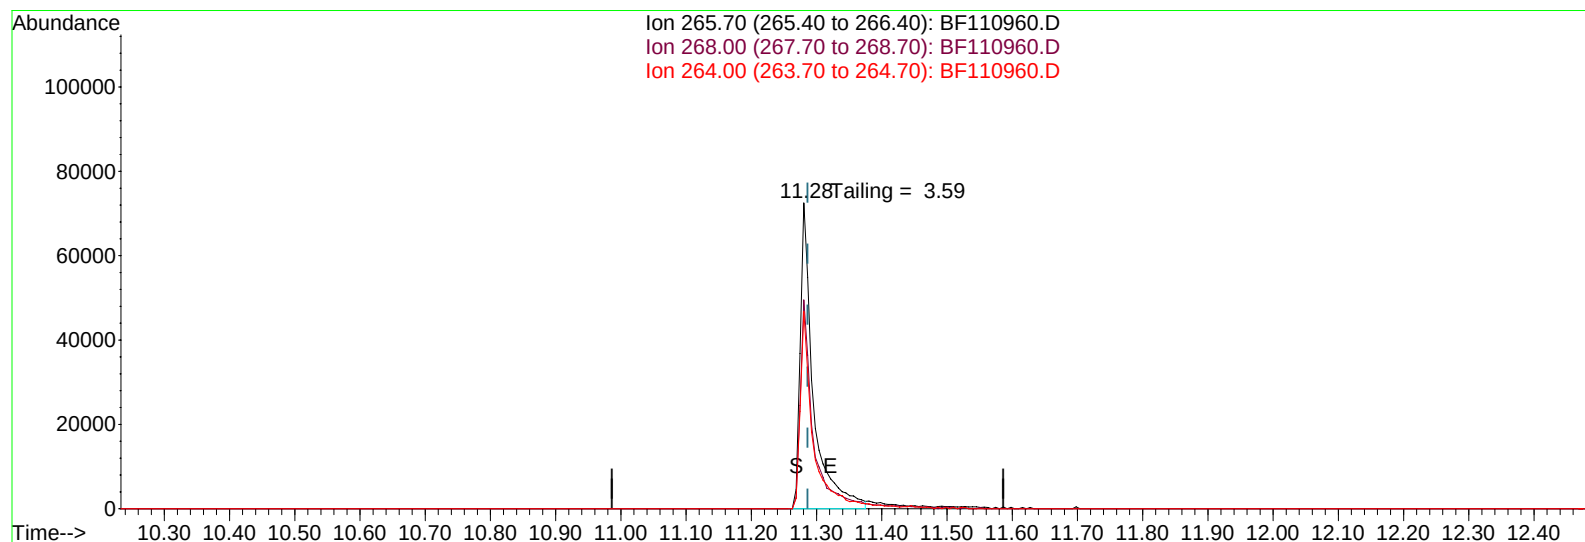

TIC: BF110960.D

(70) Pentachlorophenol (C)

11.280min (-0.006) 163836.31ng

response 108127

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.31
264.00	63.20	64.51
0.00	0.00	0.00