


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112618\  
 Data File : BF110951.D  
 Acq On : 26 Nov 2018 9:10  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF112618.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Nov 27 06:43:50 2018

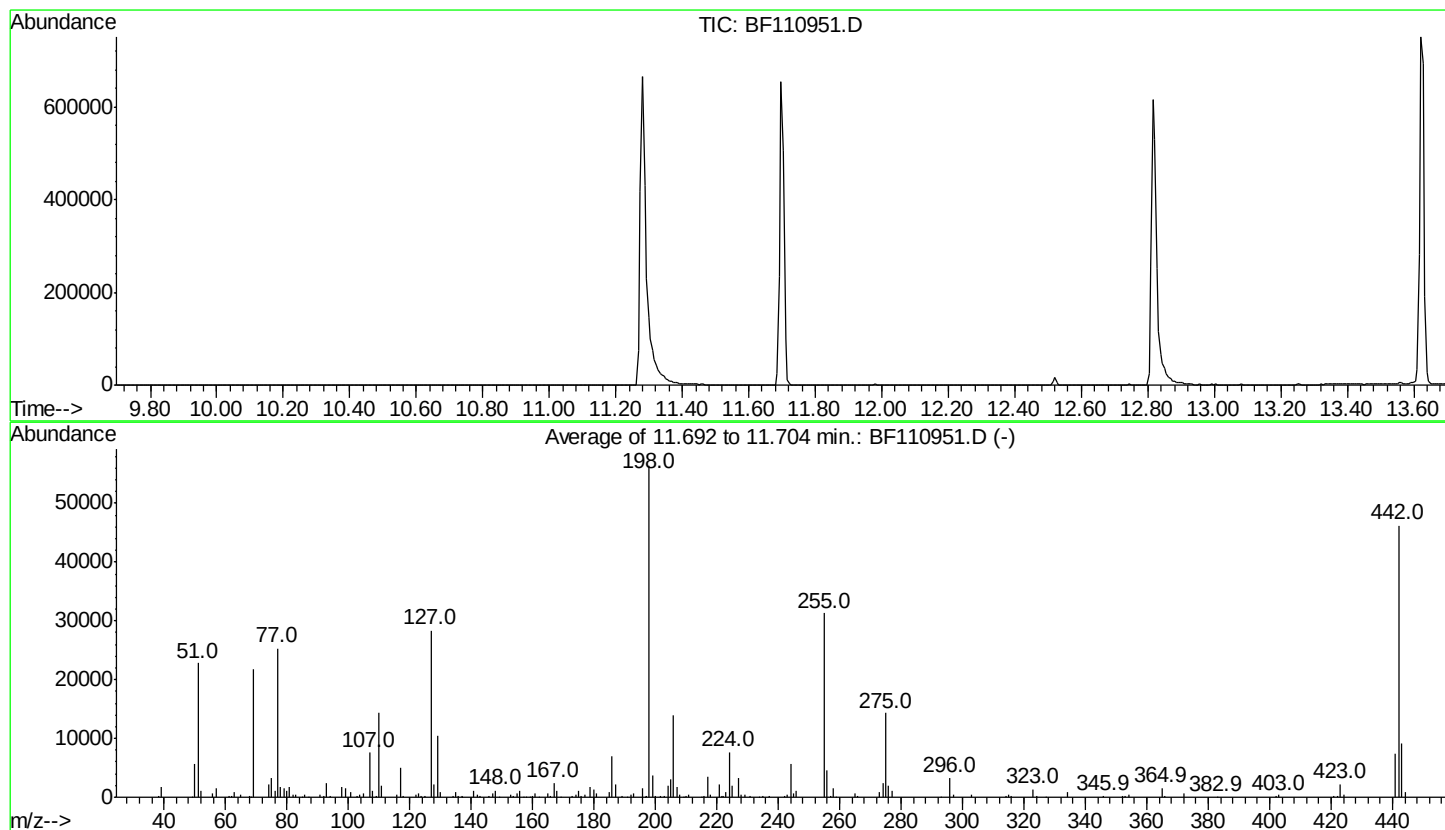

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.5      | 22848   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.7       | 162     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.5      | 21700   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 50.3      | 28392   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 248     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 56421   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 3723    | PASS             |
| 275         | 198          | 10           | 60           | 25.3      | 14294   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 1532    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.3      | 7504    | PASS             |
| 442         | 198          | 50           | 100          | 82.0      | 46288   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 9087    | PASS             |