


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112618\
 Data File : BF110960.D
 Acq On : 26 Nov 2018 13:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 27 06:43:50 2018

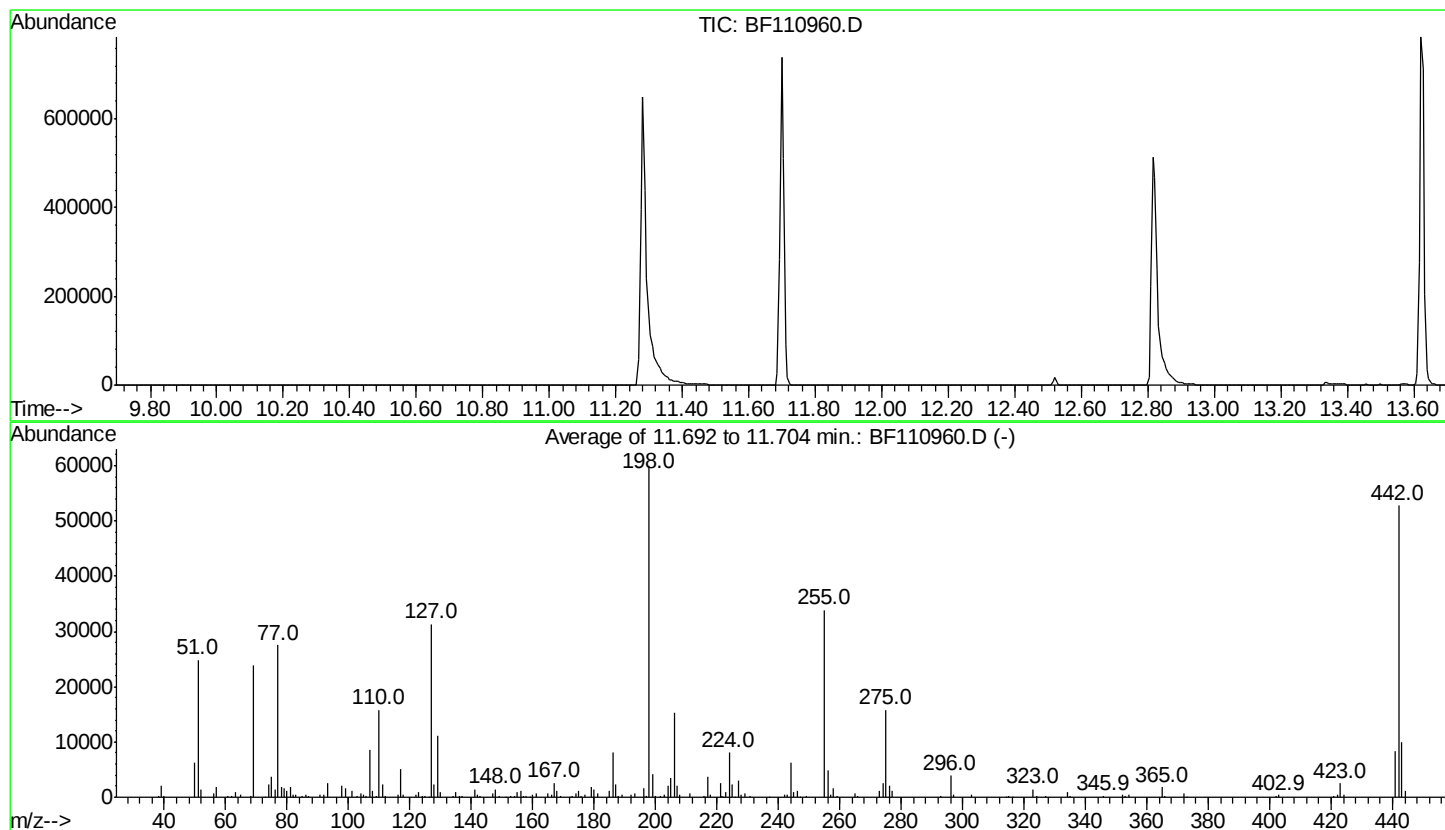

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	24902	PASS
68	69	0.00	2	1.3	301	PASS
69	198	0.00	100	39.9	23955	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	31282	PASS
197	198	0.00	2	0.4	247	PASS
198	198	100	100	100.0	60008	PASS
199	198	5	9	6.9	4147	PASS
275	198	10	60	26.3	15772	PASS
365	198	1	100	3.0	1807	PASS
441	198	0.01	100	13.8	8307	PASS
442	198	50	100	87.9	52773	PASS
443	442	15	24	18.8	9933	PASS