


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112618\
 Data File : BF110986.D
 Acq On : 27 Nov 2018 2:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 27 06:43:50 2018

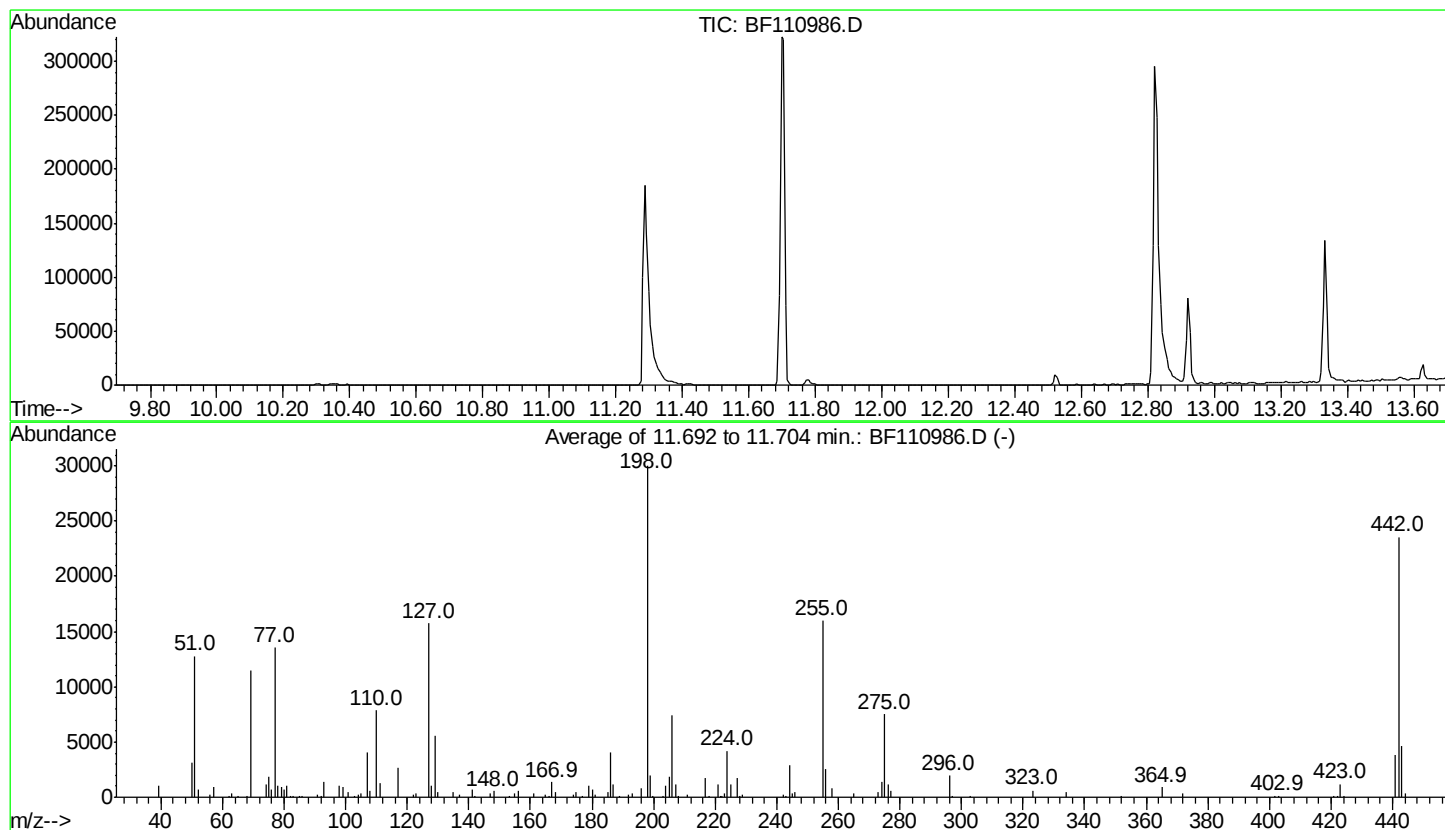

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	12794	PASS
68	69	0.00	2	0.9	104	PASS
69	198	0.00	100	38.1	11443	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	15713	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30029	PASS
199	198	5	9	6.6	1989	PASS
275	198	10	60	25.0	7518	PASS
365	198	1	100	3.1	918	PASS
441	198	0.01	100	12.7	3801	PASS
442	198	50	100	78.5	23561	PASS
443	442	15	24	19.9	4683	PASS