


Data Path : Z:\HPCHEM1\BNA_F\Data\BF010215\
 Data File : BF076723.D
 Acq On : 2 Jan 2015 11:56
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 26 13:50:53 2014

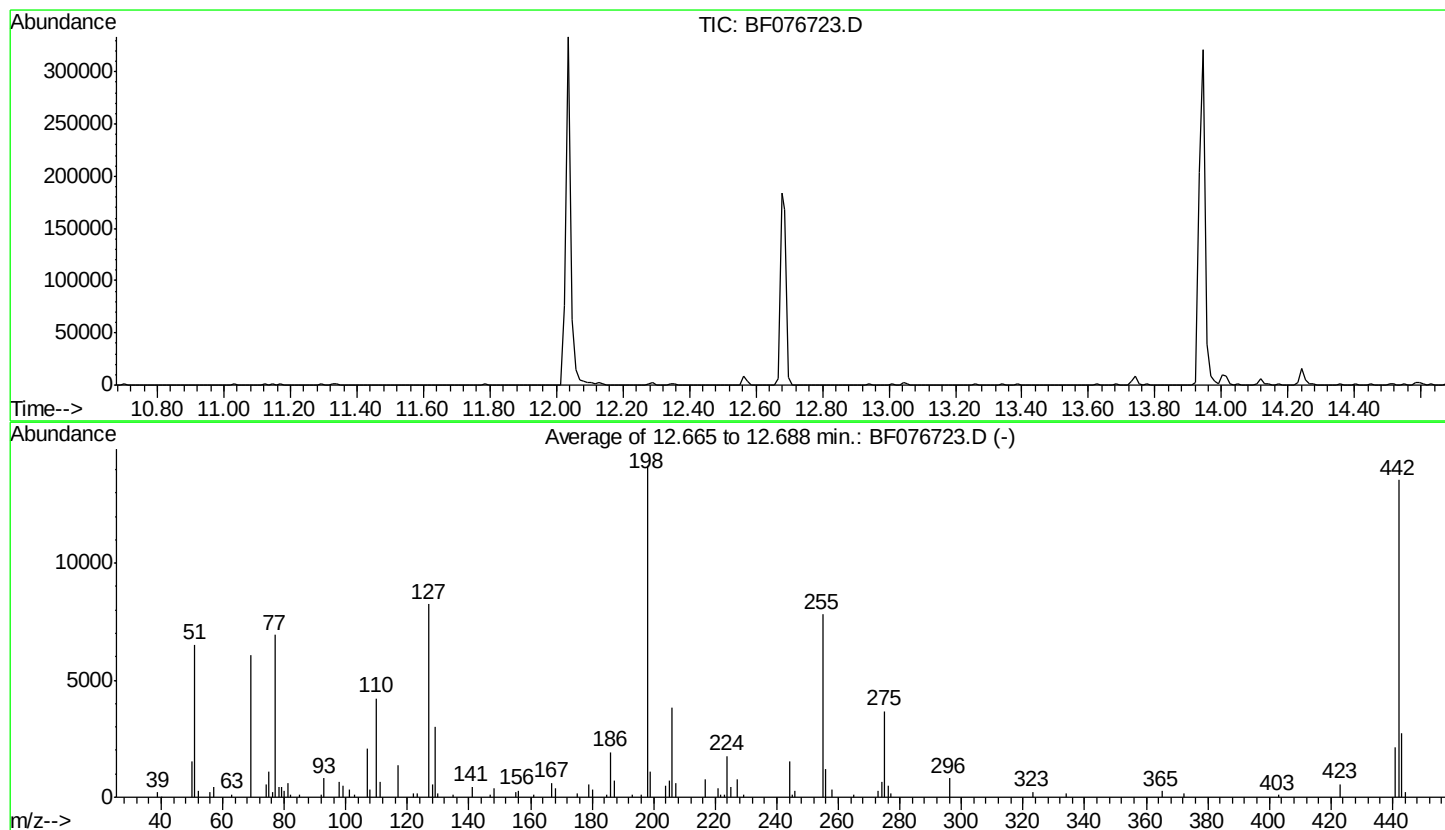

AutoFind: Scans 1013, 1014, 1015; Background Corrected with Scan 1010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	6534	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.0	6099	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.3	8257	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14169	PASS
199	198	5	9	7.7	1086	PASS
275	198	10	60	25.9	3676	PASS
365	198	1	100	1.9	267	PASS
441	442	0.01	24	15.9	2160	PASS
442	198	50	100	95.7	13556	PASS
443	442	15	24	20.0	2711	PASS