
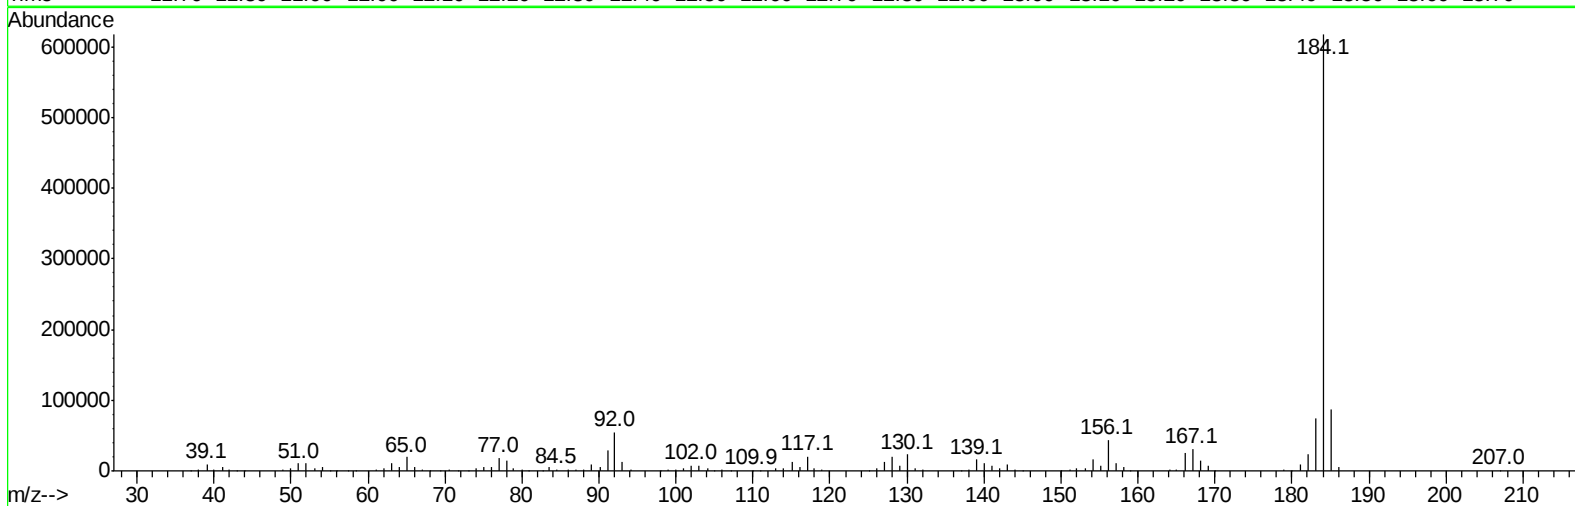


Data Path : Z:\HPCHEM1\BNA F\Data\BF010218\
Data File : BF101841.D
Acq On : 2 Jan 2018 10:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 03:00:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

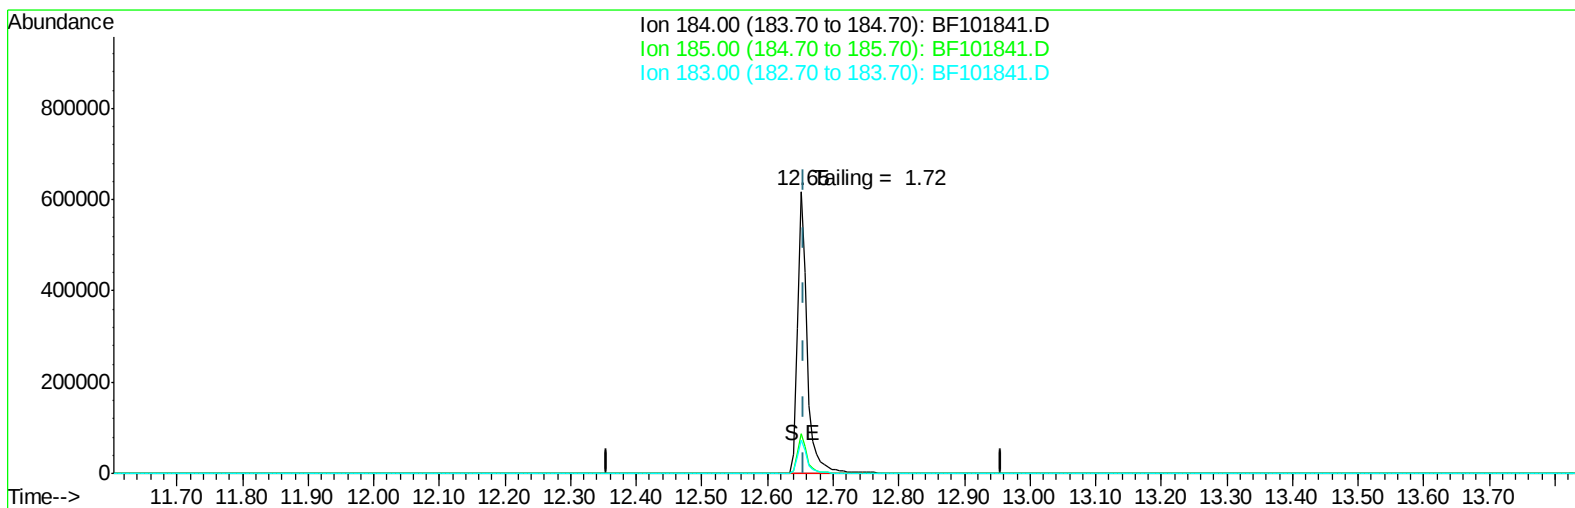

TIC: BF101841.D

(76) Benzidine



12.651min (-0.006) 52080.86ng

response 635697

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.13
183.00	11.60	11.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF010218\
Data File : BF101841.D
Acq On : 2 Jan 2018 10:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 03:00:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 13:21:45 2017
Response via : Initial Calibration

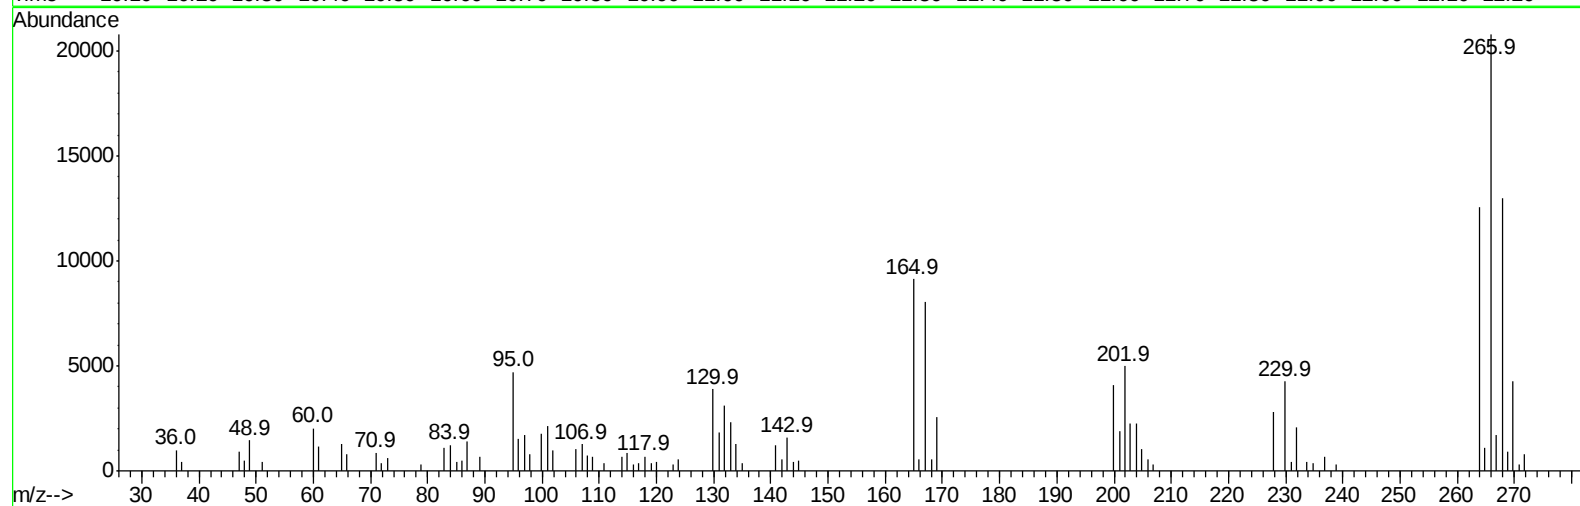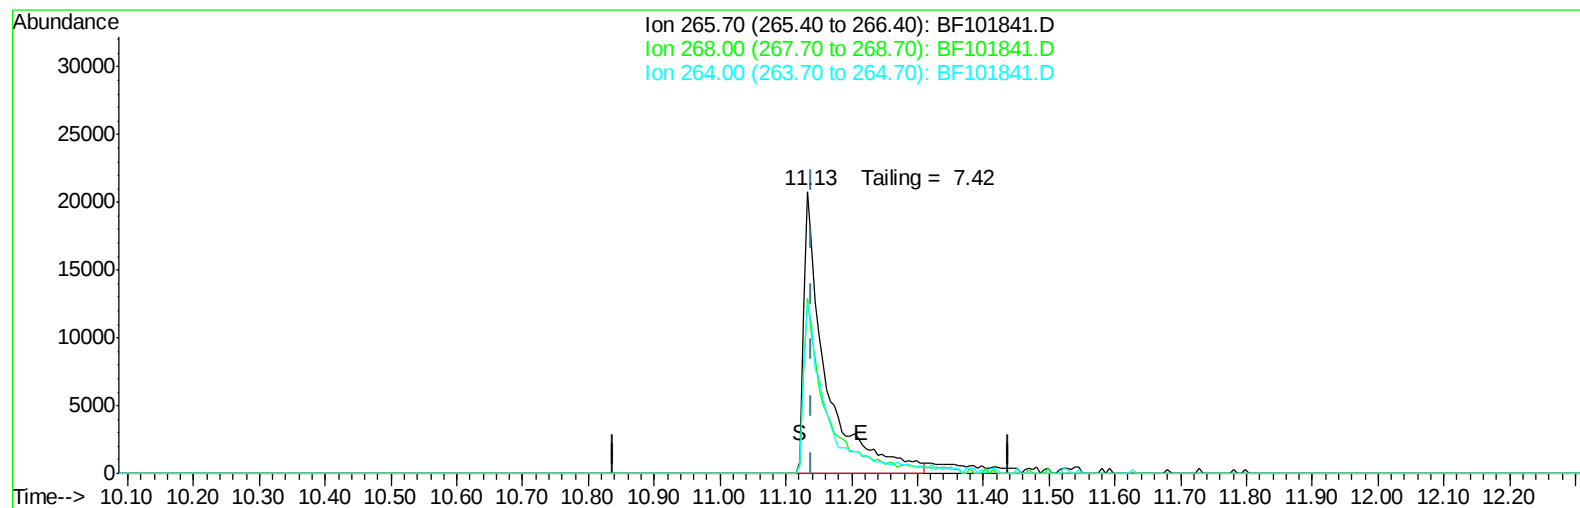

TIC: BF101841.D

(69) Pentachlorophenol (C)

11.133min (-0.006) 30510.49ng

response 48557

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.45
264.00	61.90	60.50
0.00	0.00	0.00