


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010218\
 Data File : BF101841.D
 Acq On : 2 Jan 2018 10:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 13:21:45 2017

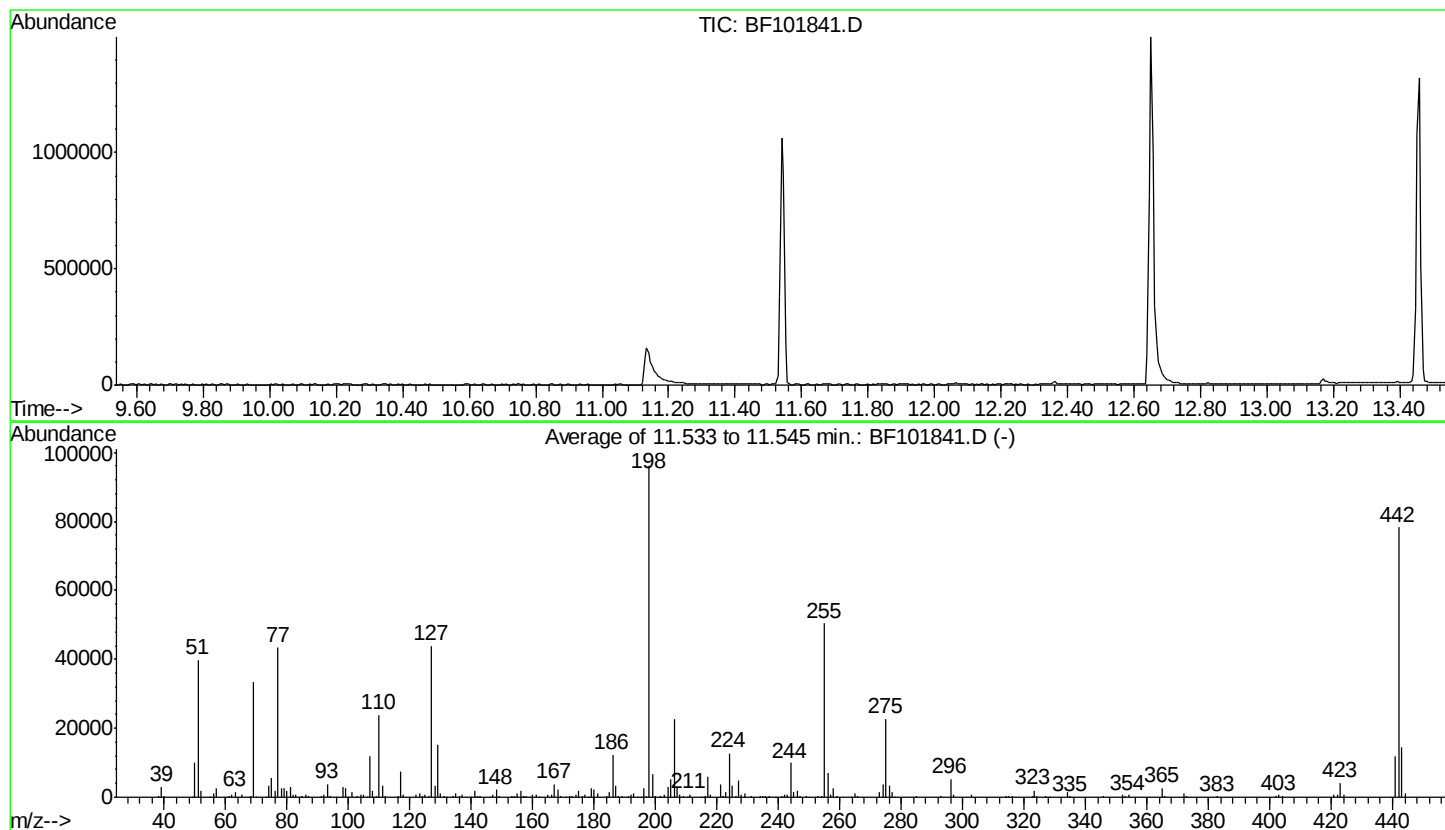

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	39924	PASS
68	69	0.00	2	1.4	472	PASS
69	198	0.00	100	34.9	33608	PASS
70	69	0.00	2	0.3	112	PASS
127	198	10	80	45.7	43925	PASS
197	198	0.00	2	0.5	523	PASS
198	198	100	100	100.0	96184	PASS
199	198	5	9	7.0	6725	PASS
275	198	10	60	23.7	22798	PASS
365	198	1	100	2.8	2729	PASS
441	443	0.01	100	81.5	11928	PASS
442	198	50	100	81.3	78210	PASS
443	442	15	24	18.7	14635	PASS